

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102821\
 Data File : VU045436.D
 Acq On : 28 Oct 2021 13:49
 Operator : SY/MD
 Sample : VU1028WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

Signal : TIC: VU045436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.517	51	55	64	rVB2	7206	7800	0.55%	0.074%
2	1.597	73	80	93	rBV	183658	205162	14.45%	1.947%
3	1.912	169	178	196	rVB	123496	152775	10.76%	1.450%
4	2.478	351	354	358	rBV3	200	170	0.01%	0.002%
5	2.501	358	361	363	rBV2	199	145	0.01%	0.001%
6	2.565	369	381	407	rBV	285866	476563	33.56%	4.522%
7	2.793	441	452	462	rBV	2113	3758	0.26%	0.036%
8	2.964	493	505	518	rBV2	584	1170	0.08%	0.011%
9	3.047	522	531	541	rBV3	2093	3580	0.25%	0.034%
10	3.118	549	553	555	rBV	141	116	0.01%	0.001%
11	3.221	582	585	590	rBV2	162	184	0.01%	0.002%
12	3.356	621	627	634	rVB3	915	1254	0.09%	0.012%
13	3.414	640	645	648	rBV2	108	119	0.01%	0.001%
14	3.565	689	692	697	rVB2	186	167	0.01%	0.002%
15	3.864	782	785	789	rBV	159	129	0.01%	0.001%
16	4.073	845	850	852	rBV	171	184	0.01%	0.002%
17	4.105	857	860	865	rVB	148	140	0.01%	0.001%
18	4.186	880	885	889	rBV2	123	110	0.01%	0.001%
19	4.272	906	912	915	rBV2	102	129	0.01%	0.001%
20	4.327	923	929	936	rVV	133	158	0.01%	0.001%
21	4.629	1005	1023	1054	rBV	142529	349918	24.64%	3.320%
22	4.928	1112	1116	1122	rBV2	290	275	0.02%	0.003%
23	5.067	1142	1159	1180	rBV	250746	541974	38.17%	5.143%
24	5.292	1223	1229	1236	rBV2	603	983	0.07%	0.009%
25	5.378	1252	1256	1257	rBV3	321	174	0.01%	0.002%
26	5.391	1257	1260	1264	rVB2	224	193	0.01%	0.002%
27	5.526	1300	1302	1306	rVB3	266	165	0.01%	0.002%
28	5.552	1306	1310	1314	rBV	103	104	0.01%	0.001%
29	5.726	1342	1364	1391	rBV2	530910	1420033	100.00%	13.475%
30	5.970	1435	1440	1444	rBV	494	465	0.03%	0.004%
31	6.041	1457	1462	1468	rVB3	315	480	0.03%	0.005%
32	6.112	1477	1484	1485	rBV2	831	669	0.05%	0.006%
33	6.253	1513	1528	1556	rBV	416048	784672	55.26%	7.446%
34	6.536	1606	1616	1630	rVB6	2947	5988	0.42%	0.057%
35	6.591	1630	1633	1634	rBV2	325	170	0.01%	0.002%
36	6.604	1635	1637	1642	rVB3	444	298	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102821\
 Data File : VU045436.D
 Acq On : 28 Oct 2021 13:49
 Operator : SY/MD
 Sample : VU1028WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

37	6.694	1650	1665	1686	rBV	333874	649277	45.72%	6.161%
38	6.803	1695	1699	1701	rBV3	737	629	0.04%	0.006%
39	6.909	1728	1732	1735	rVB2	181	131	0.01%	0.001%
40	6.935	1735	1740	1743	rBV	109	108	0.01%	0.001%
41	7.034	1768	1771	1773	rBV2	313	228	0.02%	0.002%
42	7.182	1808	1817	1826	rVV3	2795	5033	0.35%	0.048%
43	7.446	1895	1899	1902	rBV	123	113	0.01%	0.001%
44	7.568	1924	1937	1957	rVV	187111	324913	22.88%	3.083%
45	7.687	1966	1974	1983	rVB3	1988	3203	0.23%	0.030%
46	7.742	1988	1991	1997	rVB2	124	111	0.01%	0.001%
47	7.800	2001	2009	2013	rBV5	839	1044	0.07%	0.010%
48	7.845	2018	2023	2024	rBV2	132	114	0.01%	0.001%
49	7.899	2026	2040	2056	rBV	635293	1090973	76.83%	10.352%
50	8.076	2092	2095	2100	rBV2	169	157	0.01%	0.001%
51	8.182	2115	2128	2144	rBV	129533	215577	15.18%	2.046%
52	8.378	2187	2189	2194	rVB2	186	136	0.01%	0.001%
53	8.475	2212	2219	2222	rBV2	316	462	0.03%	0.004%
54	8.552	2240	2243	2250	rVB3	670	717	0.05%	0.007%
55	8.639	2256	2270	2301	rBV	438246	783000	55.14%	7.430%
56	8.922	2355	2358	2363	rBV2	418	396	0.03%	0.004%
57	8.976	2372	2375	2381	rVB2	154	142	0.01%	0.001%
58	9.015	2381	2387	2389	rBV	143	176	0.01%	0.002%
59	9.420	2500	2513	2543	rVV	564997	930431	65.52%	8.829%
60	9.574	2553	2561	2568	rVB	1177	1517	0.11%	0.014%
61	9.697	2591	2599	2609	rVB3	1744	2620	0.18%	0.025%
62	9.780	2622	2625	2629	rBV	147	105	0.01%	0.001%
63	9.999	2689	2693	2698	rBV2	269	267	0.02%	0.003%
64	10.111	2719	2728	2737	rBV6	2036	3417	0.24%	0.032%
65	10.301	2784	2787	2791	rBV	114	113	0.01%	0.001%
66	10.484	2839	2844	2852	rVB2	1055	1386	0.10%	0.013%
67	10.636	2888	2891	2894	rBV2	151	112	0.01%	0.001%
68	10.674	2895	2903	2914	rVB	3584	5094	0.36%	0.048%
69	10.761	2916	2930	2948	rBV	450146	717252	50.51%	6.806%
70	10.835	2949	2953	2956	rVB3	639	438	0.03%	0.004%
71	10.867	2959	2963	2967	rBV3	557	571	0.04%	0.005%
72	10.954	2986	2990	2994	rVB	171	143	0.01%	0.001%
73	11.092	3024	3033	3036	rBV3	946	1258	0.09%	0.012%
74	11.224	3072	3074	3079	rVB2	211	133	0.01%	0.001%
75	11.369	3116	3119	3122	rVB2	195	120	0.01%	0.001%
76	11.462	3139	3148	3160	rVB6	2882	4902	0.35%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102821\
 Data File : VU045436.D
 Acq On : 28 Oct 2021 13:49
 Operator : SY/MD
 Sample : VU1028WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

77	11.574	3180	3183	3184	rBV2	321	207	0.01%	0.002%
78	11.700	3214	3222	3230	rBV2	1536	1990	0.14%	0.019%
79	11.751	3231	3238	3245	rVB2	1676	2447	0.17%	0.023%
80	11.816	3245	3258	3272	rBV	558121	871002	61.34%	8.265%
81	11.893	3279	3282	3285	rBV2	277	188	0.01%	0.002%
82	11.980	3302	3309	3318	rVB4	2175	3288	0.23%	0.031%
83	12.070	3333	3337	3340	rBV	284	233	0.02%	0.002%
84	12.195	3356	3376	3395	rBV	582893	935655	65.89%	8.878%
85	12.333	3415	3419	3424	rVB3	473	547	0.04%	0.005%
86	12.394	3436	3438	3440	rVB	283	135	0.01%	0.001%
87	12.414	3440	3444	3447	rBV2	349	274	0.02%	0.003%
88	12.533	3478	3481	3483	rBV	248	164	0.01%	0.002%
89	13.015	3628	3631	3635	rBV	239	152	0.01%	0.001%
90	13.044	3635	3640	3642	rBV	350	335	0.02%	0.003%
91	13.063	3642	3646	3647	rBV	265	229	0.02%	0.002%
92	13.150	3667	3673	3678	rBV2	627	788	0.06%	0.007%
93	13.198	3685	3688	3690	rBV2	219	175	0.01%	0.002%
94	13.224	3690	3696	3697	rBV2	1207	1038	0.07%	0.010%
95	13.275	3709	3712	3714	rBV2	229	142	0.01%	0.001%
96	13.844	3883	3889	3897	rVB4	2269	3152	0.22%	0.030%
97	14.095	3959	3967	3978	rVB2	2856	4569	0.32%	0.043%
98	14.336	4034	4042	4048	rVB6	1987	2710	0.19%	0.026%
99	14.581	4111	4118	4129	rBV2	1009	1954	0.14%	0.019%
100	15.851	4511	4513	4514	rBV	551	243	0.02%	0.002%




Sum of corrected areas: 10538510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102821\
Data File : VU045436.D
Acq On : 28 Oct 2021 13:49
Operator : SY/MD
Sample : VU1028WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK032

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

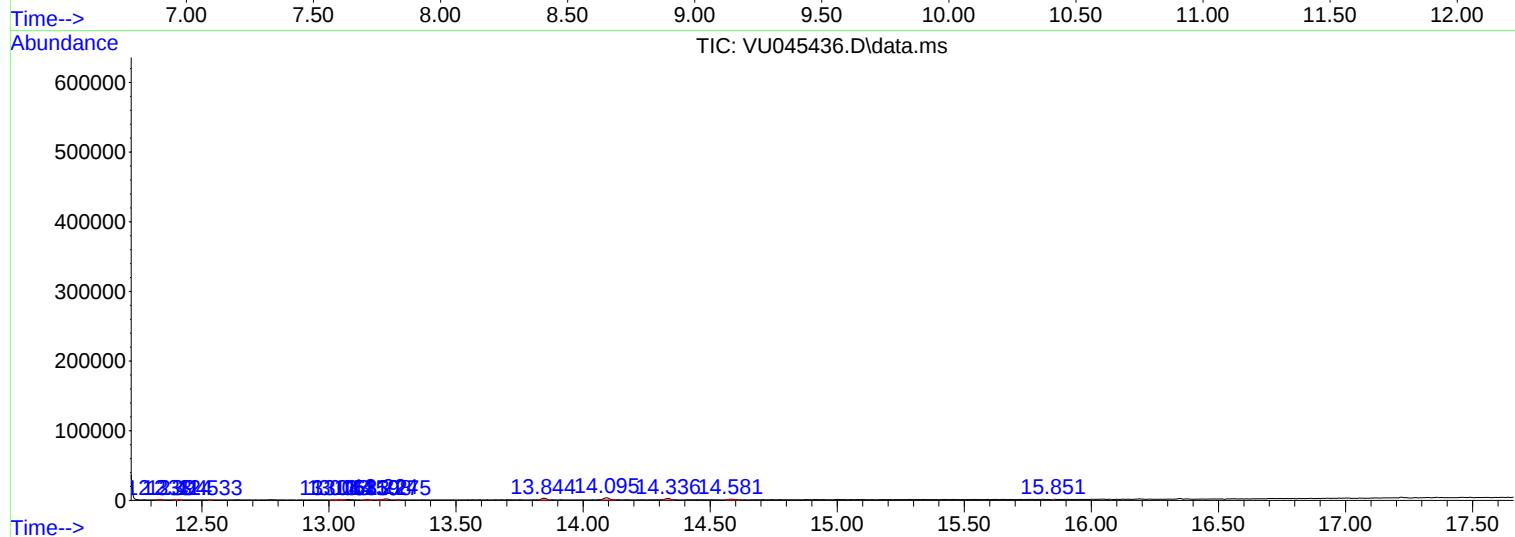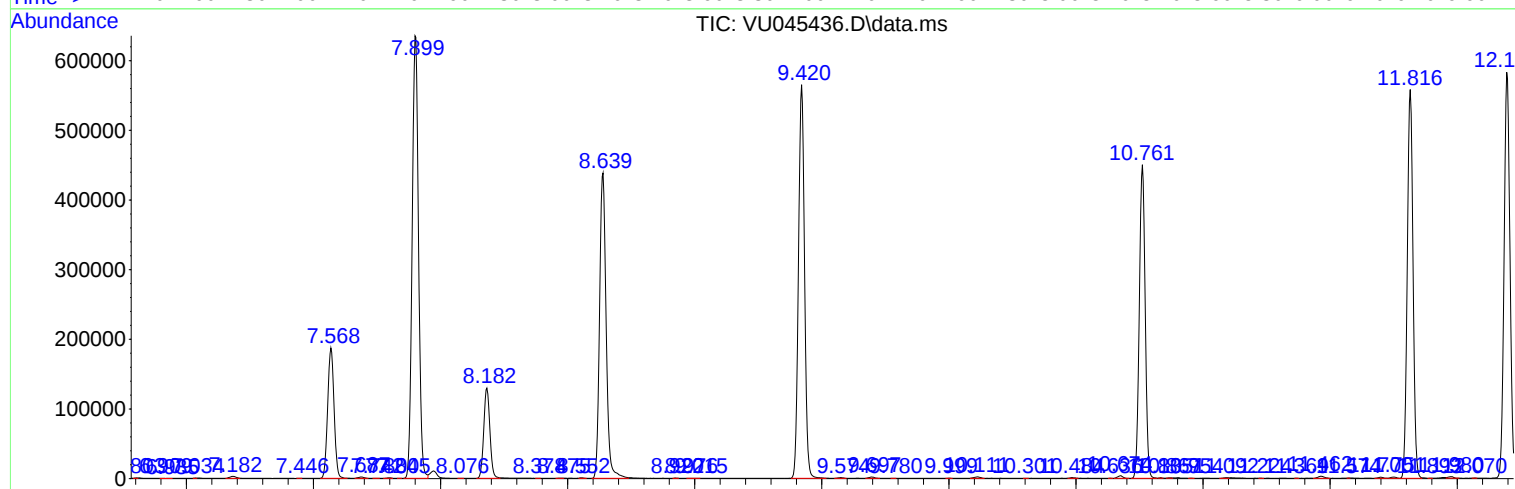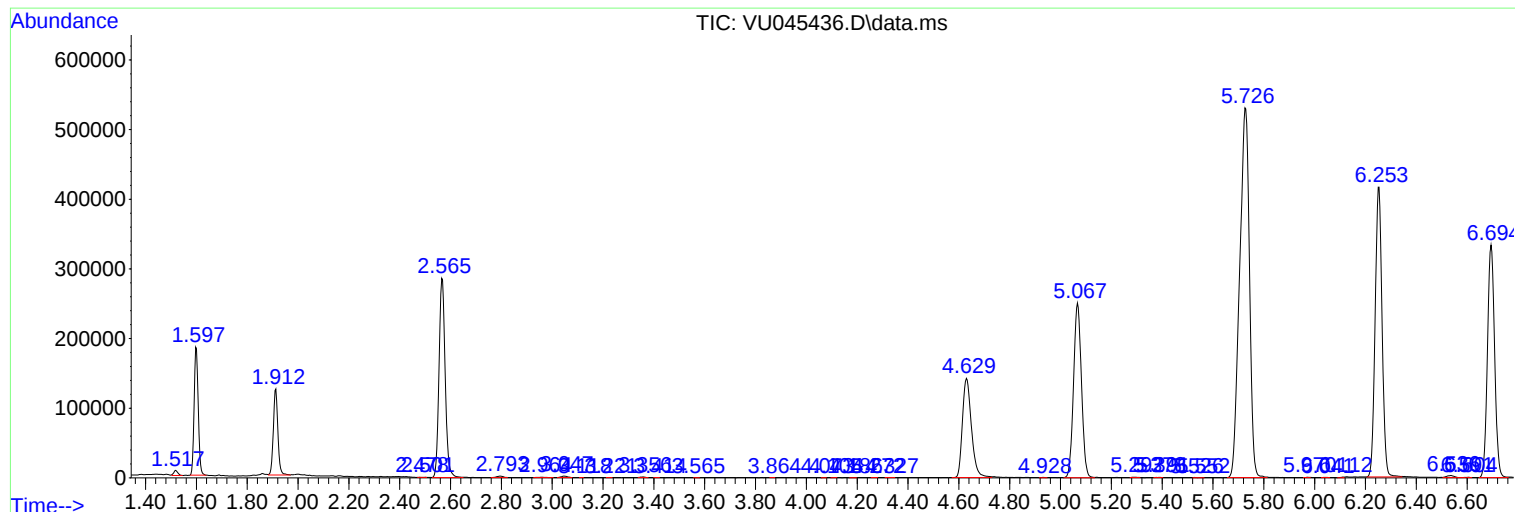

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102821\
Data File : VU045436.D
Acq On : 28 Oct 2021 13:49
Operator : SY/MD
Sample : VU1028WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK032

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102821\
Data File : VU045436.D
Acq On : 28 Oct 2021 13:49
Operator : SY/MD
Sample : VU1028WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK032

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
