


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102821\
 Data File : VU045429.D
 Acq On : 28 Oct 2021 09:11
 Operator : SY/MD
 Sample : BFB016
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB016

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis
 Last Update : Tue Nov 02 02:33:37 2021

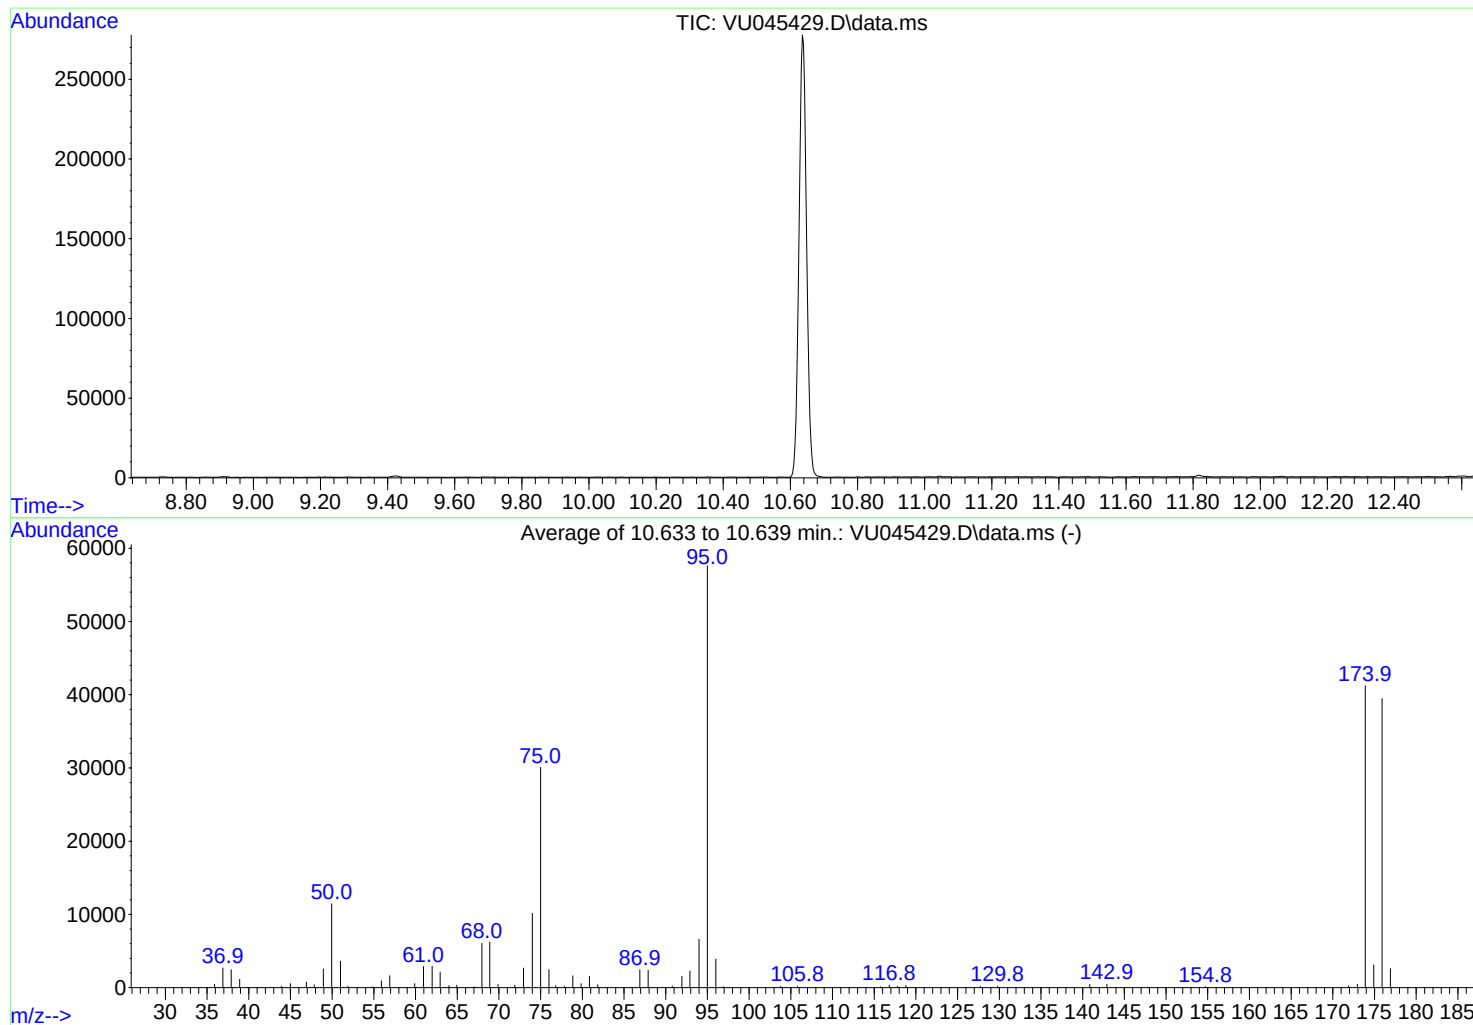

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	11454	PASS
75	95	30	80	52.2	30077	PASS
95	95	100	100	100.0	57597	PASS
96	95	5	9	6.8	3920	PASS
173	174	0.00	2	1.0	428	PASS
174	95	50	120	71.6	41224	PASS
175	174	5	9	7.5	3096	PASS
176	174	95	101	95.7	39469	PASS
177	176	5	9	6.6	2593	PASS

Scan 2878 (10.594 min): VU045429.D\data.ms
BFB016

m/z	Abundance
39.80	137.0
43.90	325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	468.0
36.90	2617.0
37.90	2404.0
38.90	1149.0
39.80	197.0
43.90	496.0
45.00	543.0
46.90	710.0
47.90	373.0
48.90	2511.0
50.00	11174.0
51.00	3490.0
51.90	173.0
54.80	139.0
55.90	933.0
56.90	1588.0
59.90	529.0
61.00	2756.0
62.00	2847.0
63.00	2026.0
64.00	287.0
65.00	346.0
66.90	184.0
67.90	5930.0
68.90	6089.0
69.90	444.0
71.90	314.0
72.90	2576.0
74.00	9882.0
75.00	29312.0
76.00	2527.0
76.80	254.0
77.90	202.0
78.90	1527.0
79.90	546.0
80.90	1480.0
81.80	364.0
86.90	2417.0
87.90	2190.0
90.80	221.0
91.90	1558.0
92.90	2093.0
94.00	6176.0
95.00	55264.0
96.00	3765.0
96.90	125.0
103.80	151.0
105.80	193.0
115.80	128.0
116.80	301.0
117.80	189.0
118.80	293.0
127.70	154.0
129.80	186.0
140.90	379.0
142.90	436.0
154.70	115.0
171.90	259.0
173.00	441.0
173.90	38704.0
174.90	2843.0
175.90	36408.0
176.90	2517.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	475.0
36.90	2775.0
37.90	2543.0
38.90	1180.0
39.80	183.0
43.90	531.0
45.00	548.0
46.90	769.0
47.90	394.0
49.00	2606.0
49.90	11797.0
51.00	3744.0
51.90	202.0
54.90	133.0
55.90	975.0
56.90	1683.0
59.90	556.0
60.90	2971.0
62.00	3031.0
62.90	2157.0
64.00	300.0
64.90	321.0
67.10	188.0
68.00	6299.0
68.90	6404.0
69.90	452.0
71.90	326.0
73.00	2781.0
74.00	10489.0
75.00	31064.0
76.00	2547.0
76.80	258.0
77.80	212.0
78.80	1671.0
79.80	577.0
80.80	1589.0
81.90	400.0
85.80	101.0
86.90	2469.0
87.90	2442.0
90.80	227.0
91.90	1577.0
92.90	2335.0
94.00	6859.0
95.00	59488.0
96.00	4042.0
96.90	145.0
103.80	180.0
105.80	220.0
115.80	145.0
116.80	349.0
117.80	210.0
118.80	323.0
127.70	153.0
129.80	191.0
140.90	464.0
142.90	461.0
147.80	113.0
154.80	122.0
171.90	268.0
172.90	440.0
173.90	42504.0
174.90	3238.0
175.90	40880.0
176.90	2674.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016

m/z	Abundance
35.90	418.0
36.90	2687.0
37.90	2419.0
38.90	1053.0
39.80	197.0
43.90	560.0
45.00	516.0
46.90	748.0
47.80	384.0
49.00	2466.0
49.90	11390.0
51.00	3663.0
51.90	196.0
55.00	135.0
55.90	920.0
56.90	1613.0
59.90	566.0
60.90	2943.0
62.00	2886.0
62.90	2152.0
64.00	267.0
64.90	286.0
67.10	159.0
68.00	5976.0
68.90	6103.0
69.90	449.0
71.90	323.0
73.00	2641.0
74.00	10041.0
75.00	29856.0
76.00	2312.0
76.80	277.0
77.80	214.0
78.80	1667.0
79.90	529.0
80.80	1550.0
81.80	396.0
86.90	2417.0
87.90	2421.0
90.80	199.0
92.00	1499.0
92.90	2407.0
94.00	6778.0
95.00	58040.0
96.00	3952.0
96.90	144.0
103.80	185.0
105.80	213.0
115.80	146.0
116.80	360.0
117.80	196.0
118.80	282.0
127.80	158.0
129.80	193.0
140.80	474.0
142.90	454.0
147.80	131.0
154.80	134.0
171.90	246.0
172.90	404.0
173.90	42464.0
174.90	3208.0
175.90	41120.0
176.90	2588.0

Instrument :
MSVOA_U
ClientSampleId :
BFB016