




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051597.D
Acq On : 29 Oct 2022 04:00
Operator : JC/MD
Sample : N5276-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4X7

Manual IntegrationsAPPROVED

Quant Time: Oct 29 05:07:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 29 00:39:42 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/31/2022
Supervised By :Mahesh Dadoda 11/02/2022

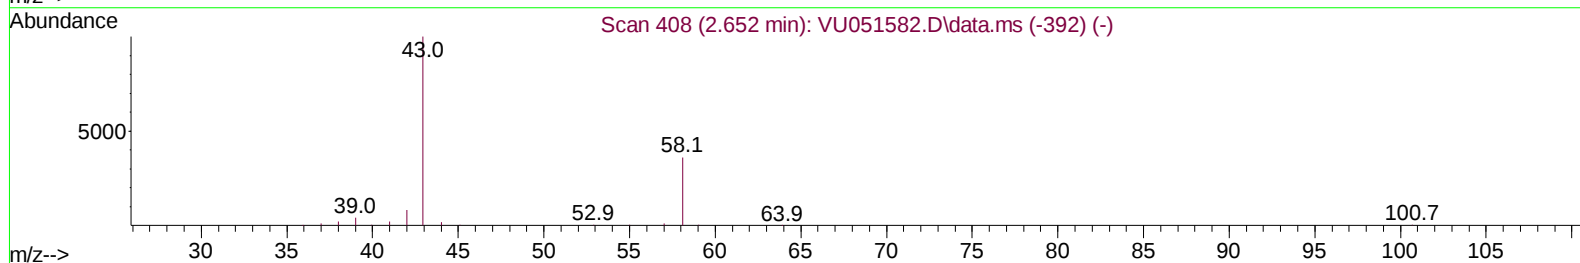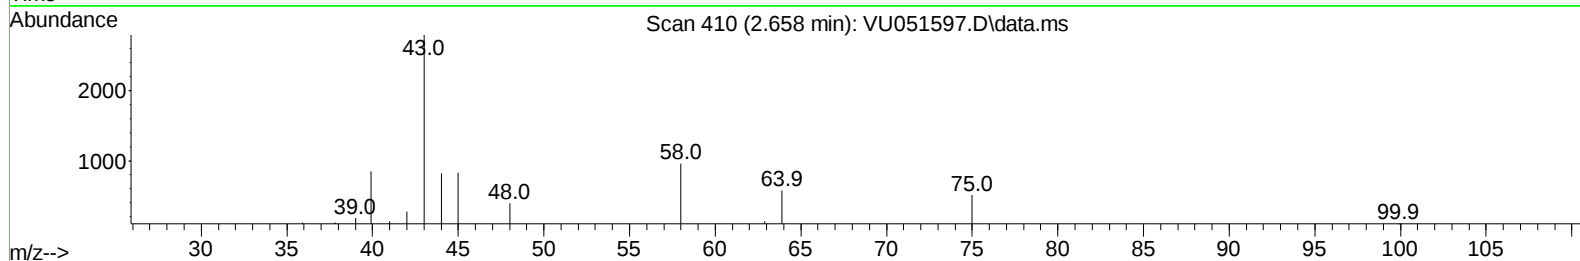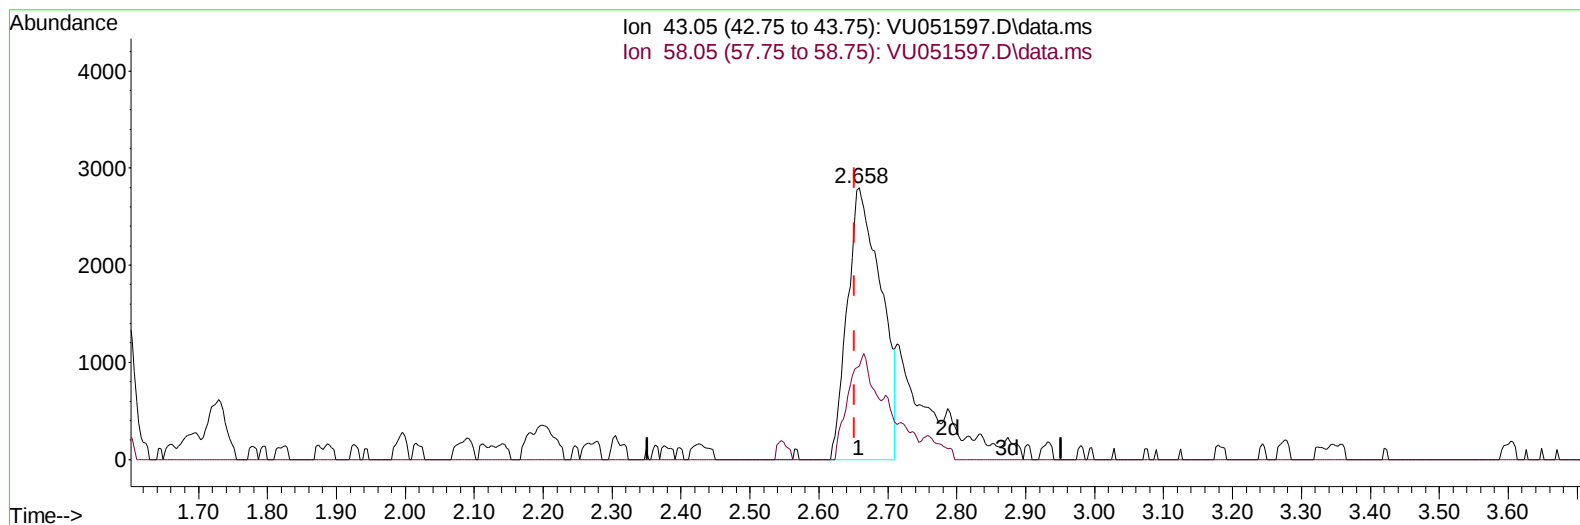

TIC: VU051597.D\data.ms

(13) Acetone (T)

2.658min (+ 0.006) 3.76 ug/L

response 9452

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.90	30.72
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051597.D
 Acq On : 29 Oct 2022 04:00
 Operator : JC/MD
 Sample : N5276-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4X7

Manual IntegrationsAPPROVED

Quant Time: Oct 29 05:07:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 29 00:39:42 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/31/2022
 Supervised By :Mahesh Dadoda 11/02/2022

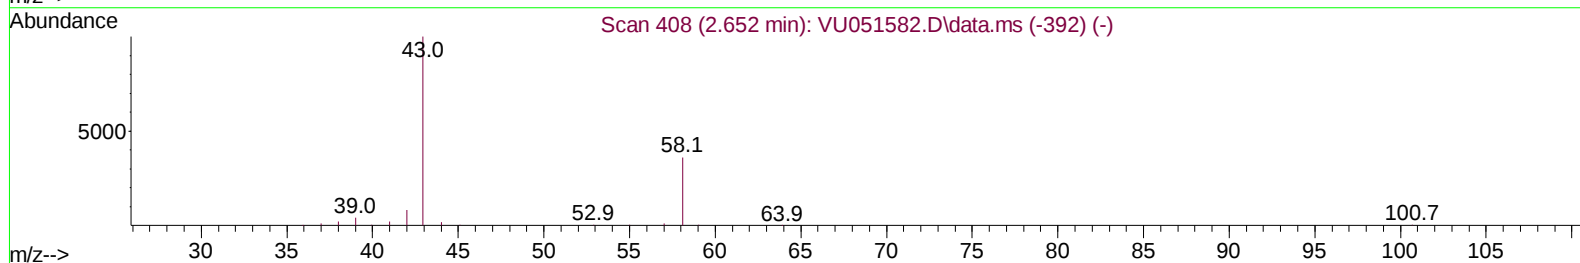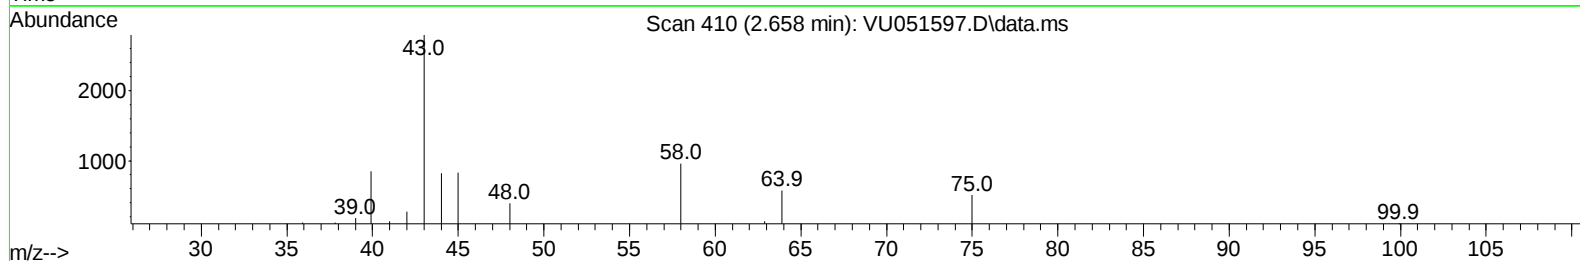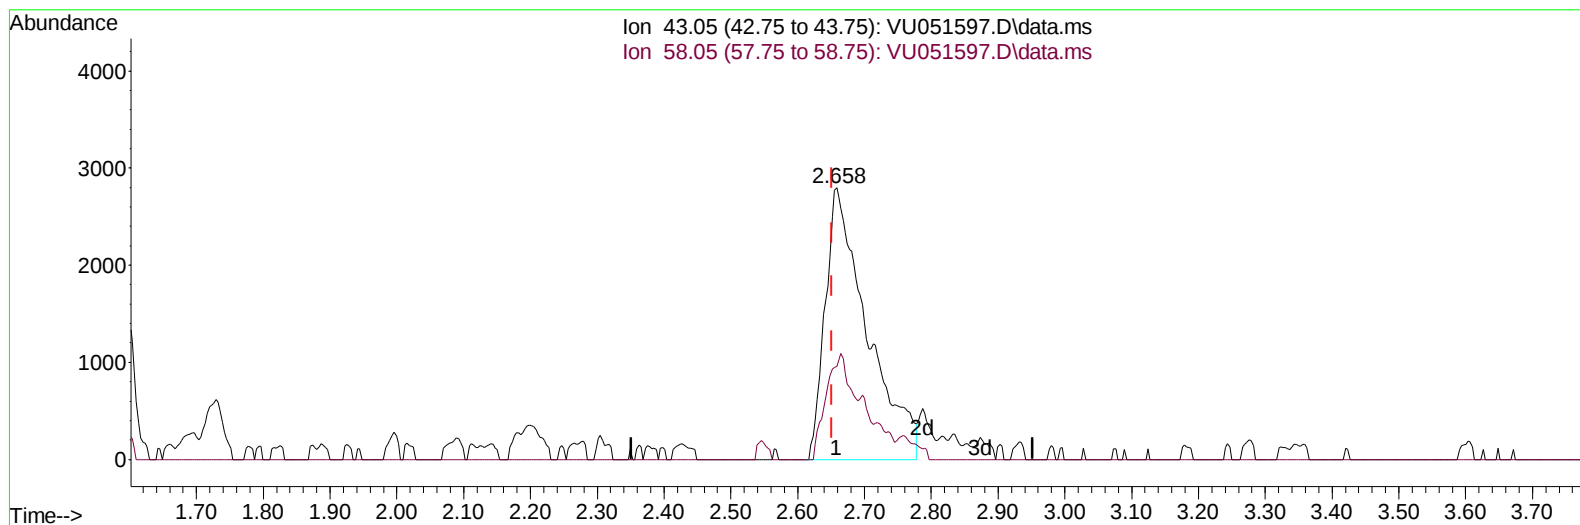

TIC: VU051597.D\data.ms

(13) Acetone (T)

2.658min (+ 0.006) 4.83 ug/L m

response 12162

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.90	23.88
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051597.D
 Acq On : 29 Oct 2022 04:00
 Operator : JC/MD
 Sample : N5276-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4X7

Manual IntegrationsAPPROVED

Quant Time: Oct 29 05:07:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 29 00:39:42 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/31/2022
 Supervised By :Mahesh Dadoda 11/02/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.247	114		181775	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117		195975	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152		80797	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.597	65		66751	4.876	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.600%	
7) Chloroethane-d5	1.912	69		74014	5.184	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.600%	
11) 1,1-Dichloroethene-d2	2.565	65		25461	5.124	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.400%	
20) 2-Butanone-d5	4.642	46		265796	53.609	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.220%	
24) Chloroform-d	5.060	84		169330	5.286	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.800%	
26) 1,2-Dichloroethane-d4	5.700	65		93137	5.382	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.600%	
32) Benzene-d6	5.726	84		295184	4.773	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	6.690	67		109250	5.052	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.000%	
41) Toluene-d8	7.896	98		201108	4.135	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.800%	
43) trans-1,3-Dichloroprop...	8.179	79		24518	3.708	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.200%	
46) 2-Hexanone-d5	8.636	63		195963	49.231	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.460%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84		100035	5.048	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.000%	
66) 1,2-Dichlorobenzene-d4	12.192	152		79970	5.393	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%	
Target Compounds							
13) Acetone	2.658	43		12162m	4.835	ug/L	
14) Carbon disulfide	2.790	76		42010	0.825	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051597.D
Acq On : 29 Oct 2022 04:00
Operator : JC/MD
Sample : N5276-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4X7

Manual IntegrationsAPPROVED

Quant Time: Oct 29 05:07:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 29 00:39:42 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/31/2022
Supervised By :Mahesh Dadoda 11/02/2022

