

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051587.D
 Acq On : 28 Oct 2022 23:48
 Operator : JC/MD
 Sample : N5276-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4W5

Quant Time: Oct 29 00:54:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 29 00:39:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	211150	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	220217	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	85823	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.594	65	66344	4.172	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.400%
7) Chloroethane-d5	1.909	69	67340	4.060	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.200%
11) 1,1-Dichloroethene-d2	2.562	65	24395	4.227	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.600%
20) 2-Butanone-d5	4.648	46	131371	22.810	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	45.620%
24) Chloroform-d	5.060	84	139446	3.747	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.000%
26) 1,2-Dichloroethane-d4	5.700	65	72073	3.585	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.800%
32) Benzene-d6	5.726	84	260321	3.746	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.000%
36) 1,2-Dichloropropane-d6	6.690	67	89307	3.675	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	73.600%
41) Toluene-d8	7.896	98	181546	3.322	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.400%#
43) trans-1,3-Dichloroprop...	8.179	79	16449	2.214	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	44.200%#
46) 2-Hexanone-d5	8.635	63	139332	31.151	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	62.300%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	78737	3.536	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	70.800%
66) 1,2-Dichlorobenzene-d4	12.192	152	72407	4.597	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.000%
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.787	76	39564	0.669	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051587.D
Acq On : 28 Oct 2022 23:48
Operator : JC/MD
Sample : N5276-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4W5

Quant Time: Oct 29 00:54:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 29 00:39:42 2022
Response via : Initial Calibration

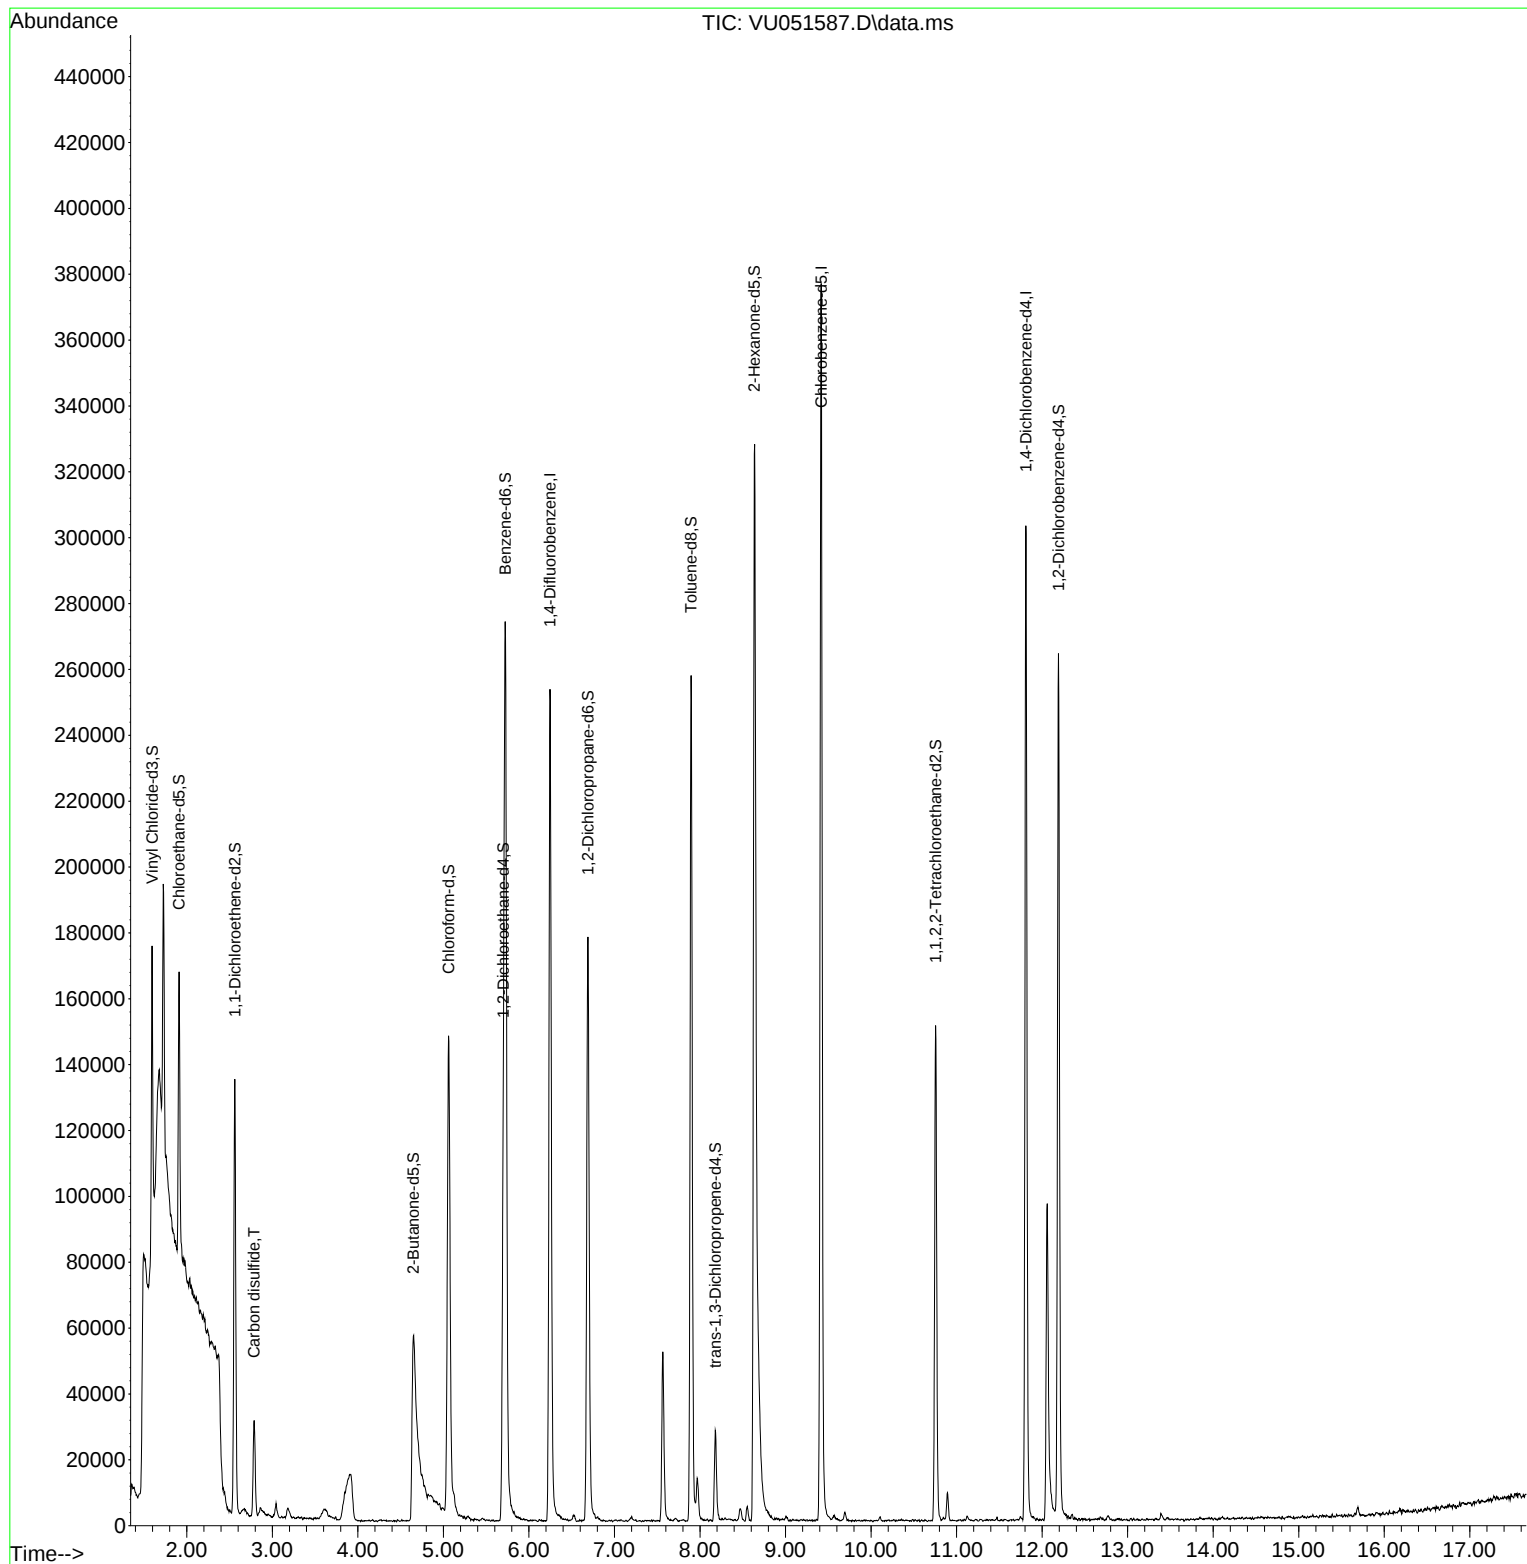

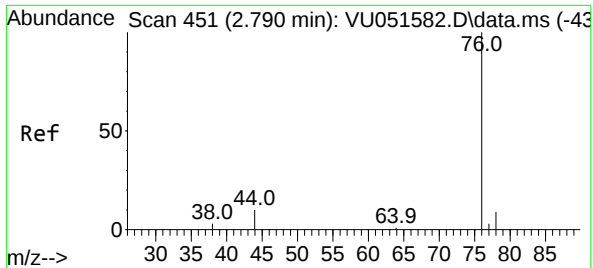

#14
Carbon disulfide
Concen: 0.669 ug/L
RT: 2.787 min Scan# 41
Delta R.T. -0.003 min
Lab File: VU051587.D
Acq: 28 Oct 2022 23:48

Instrument :
MSVOA_U
ClientSampleId :
EW4W5

Tgt Ion: 76 Resp: 39564
Ion Ratio Lower Upper
76 100
78 9.8 7.4 11.2

