

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051590.D
 Acq On : 29 Oct 2022 01:03
 Operator : JC/MD
 Sample : N5276-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4W8

Quant Time: Oct 29 04:04:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 29 00:39:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	259449	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	274963	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	107128	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	63942	3.272	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.400%
7) Chloroethane-d5	1.909	69	66089	3.243	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	64.800%#
11) 1,1-Dichloroethene-d2	2.565	65	23710	3.343	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.800%
20) 2-Butanone-d5	4.620	46	200684	28.358	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	56.720%
24) Chloroform-d	5.063	84	141330	3.091	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	61.800%#
26) 1,2-Dichloroethane-d4	5.700	65	76337	3.090	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	61.800%#
32) Benzene-d6	5.726	84	263577	3.038	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	60.800%#
36) 1,2-Dichloropropane-d6	6.687	67	93764	3.090	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	61.800%
41) Toluene-d8	7.896	98	184424	2.703	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	54.000%#
43) trans-1,3-Dichloroprop...	8.179	79	19065	2.055	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	41.200%#
46) 2-Hexanone-d5	8.632	63	140315	25.125	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	50.240%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	81843	2.944	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	58.800%#
66) 1,2-Dichlorobenzene-d4	12.192	152	68893	3.504	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	70.000%#
Target Compounds					Qvalue	
13) Acetone	2.626	43	11715	3.263	ug/L	98
14) Carbon disulfide	2.790	76	47420	0.652	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051590.D
Acq On : 29 Oct 2022 01:03
Operator : JC/MD
Sample : N5276-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4W8

Quant Time: Oct 29 04:04:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 29 00:39:42 2022
Response via : Initial Calibration

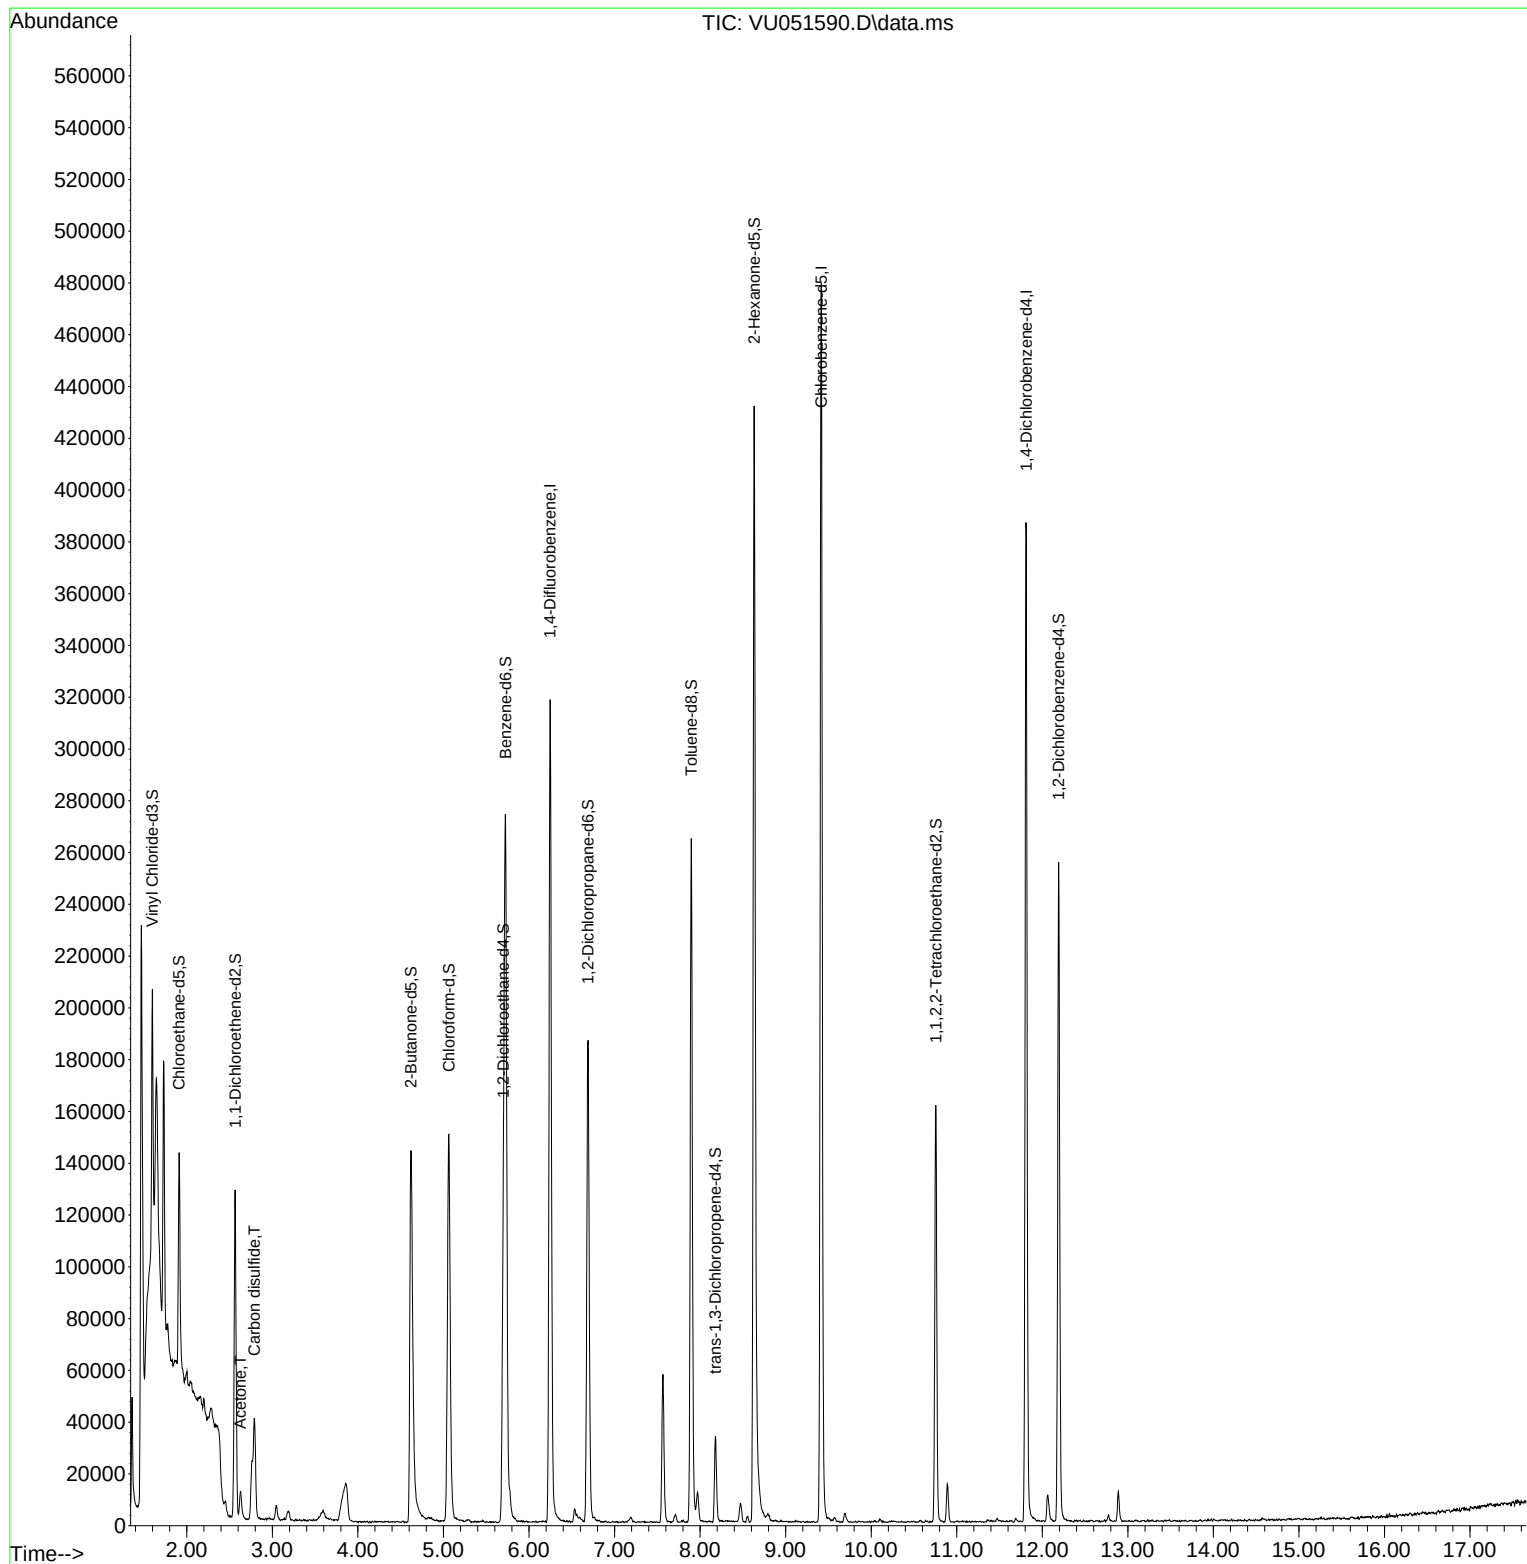

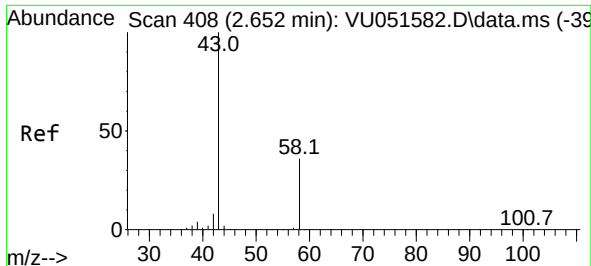

#13

Acetone

Concen: 3.263 ug/L

RT: 2.626 min Scan# 408

Delta R.T. -0.026 min

Lab File: VU051590.D

Acq: 29 Oct 2022 01:03

Instrument :

MSVOA_U

ClientSampleId :





EW4W8

Tgt Ion: 43 Resp: 11715

Ion Ratio Lower Upper

43 100

58 35.4 0.0 73.8

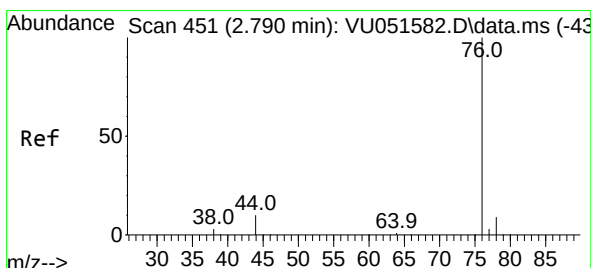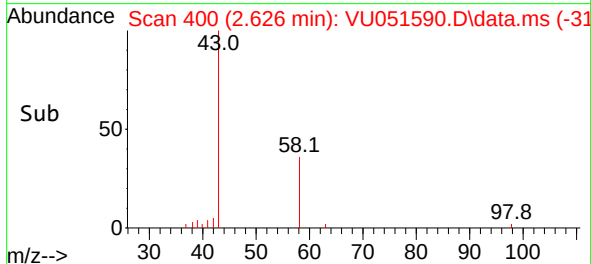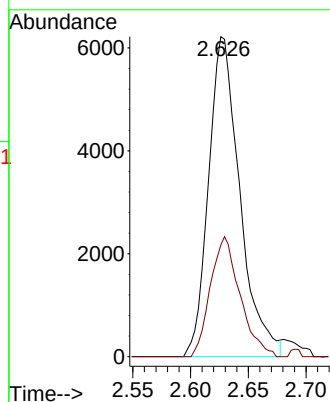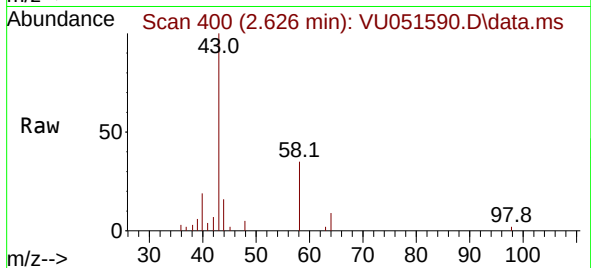

#14

Carbon disulfide

Concen: 0.652 ug/L

RT: 2.790 min Scan# 451

Delta R.T. -0.000 min

Lab File: VU051590.D

Acq: 29 Oct 2022 01:03

Tgt Ion: 76 Resp: 47420

Ion Ratio Lower Upper

76 100

78 9.8 7.4 11.2

