

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051595.D
 Acq On : 29 Oct 2022 03:09
 Operator : JC/MD
 Sample : N5276-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4X5

Quant Time: Oct 29 04:05:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 29 00:39:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	178954	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	197123	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	79224	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	64488	4.785	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.600%
7) Chloroethane-d5	1.912	69	71537	5.089	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.800%
11) 1,1-Dichloroethene-d2	2.565	65	23269	4.757	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.200%
20) 2-Butanone-d5	4.616	46	284287	58.242	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.480%
24) Chloroform-d	5.060	84	164843	5.227	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.600%
26) 1,2-Dichloroethane-d4	5.700	65	92901	5.453	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.000%
32) Benzene-d6	5.726	84	290372	4.668	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
36) 1,2-Dichloropropane-d6	6.687	67	108857	5.004	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.000%
41) Toluene-d8	7.896	98	194627	3.979	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	8.179	79	27612	4.152	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.000%
46) 2-Hexanone-d5	8.632	63	203504	50.828	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.660%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	103856	5.210	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	77364	5.320	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.400%
Target Compounds						
13) Acetone	2.623	43	12215	4.932	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051595.D
Acq On : 29 Oct 2022 03:09
Operator : JC/MD
Sample : N5276-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4X5

Quant Time: Oct 29 04:05:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 29 00:39:42 2022
Response via : Initial Calibration

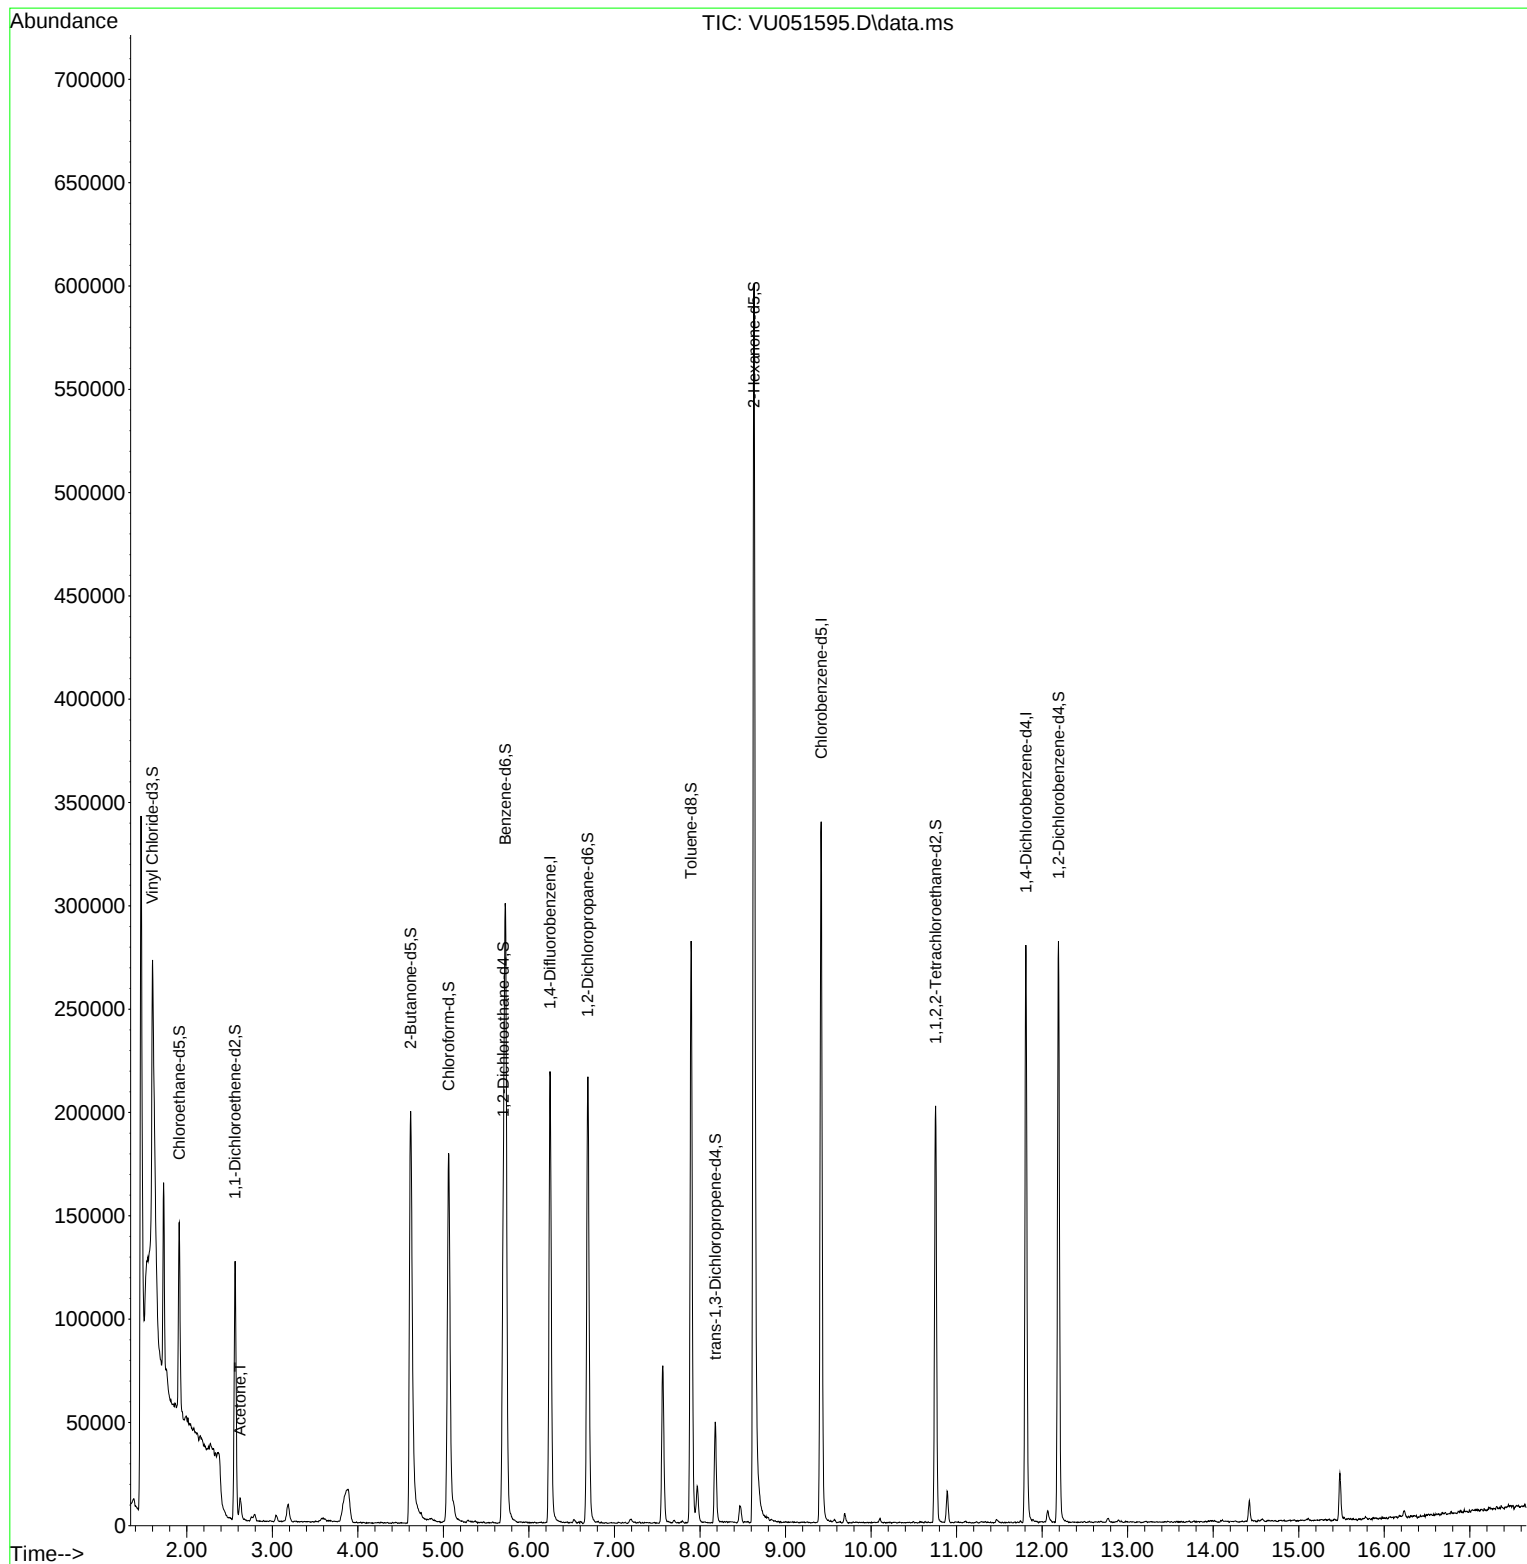

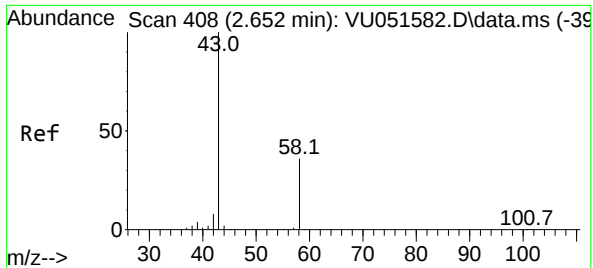

#13
 Acetone
 Concen: 4.932 ug/L
 RT: 2.623 min Scan# 31
 Delta R.T. -0.029 min
 Lab File: VU051595.D
 Acq: 29 Oct 2022 03:09

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4X5

Tgt Ion: 43 Resp: 12215
 Ion Ratio Lower Upper
 43 100
 58 34.9 0.0 73.8

