

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051596.D
 Acq On : 29 Oct 2022 03:34
 Operator : JC/MD
 Sample : N5276-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4X6

Quant Time: Oct 29 04:05:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 29 00:39:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	176345	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	196265	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	76988	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	66216	4.986	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	99.800%	
7) Chloroethane-d5	1.909	69	74484	5.377	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	107.600%	
11) 1,1-Dichloroethene-d2	2.565	65	24080	4.996	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	100.000%	
20) 2-Butanone-d5	4.617	46	284634	59.176	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	118.360%	
24) Chloroform-d	5.060	84	167463	5.388	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	107.800%	
26) 1,2-Dichloroethane-d4	5.700	65	92284	5.497	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	110.000%	
32) Benzene-d6	5.726	84	295355	4.769	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
36) 1,2-Dichloropropane-d6	6.687	67	111028	5.127	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.600%	
41) Toluene-d8	7.896	98	197294	4.051	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.000%	
43) trans-1,3-Dichloroprop...	8.179	79	27530	4.157	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.200%	
46) 2-Hexanone-d5	8.629	63	204441	51.285	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	102.580%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	105904	5.336	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	106.800%	
66) 1,2-Dichlorobenzene-d4	12.192	152	79302	5.612	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.200%	
Target Compounds						
13) Acetone	2.626	43	10237	4.195	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051596.D
Acq On : 29 Oct 2022 03:34
Operator : JC/MD
Sample : N5276-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4X6

Quant Time: Oct 29 04:05:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 29 00:39:42 2022
Response via : Initial Calibration

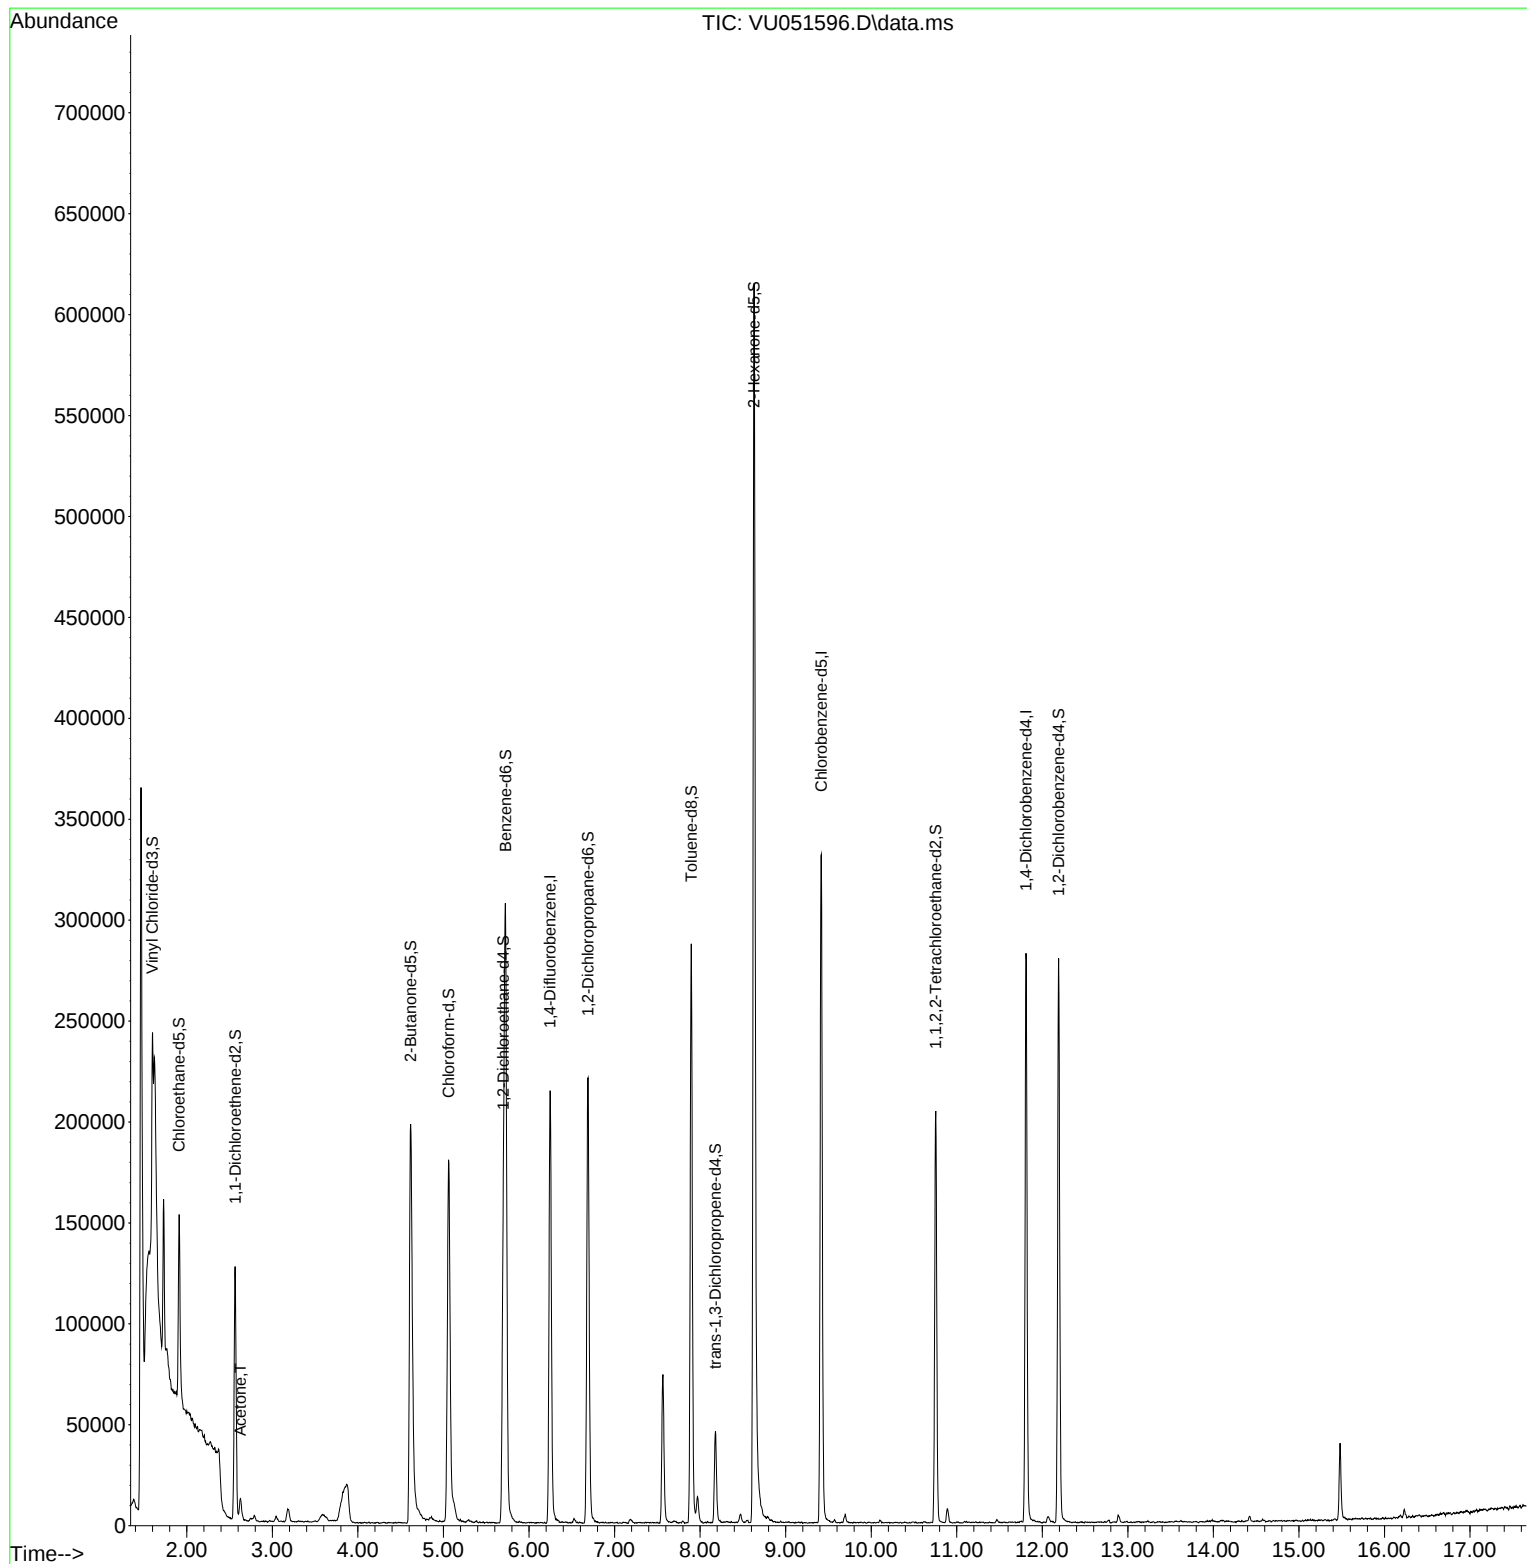

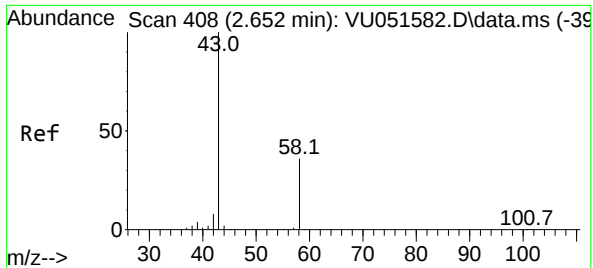

#13
 Acetone
 Concen: 4.195 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.026 min
 Lab File: VU051596.D
 Acq: 29 Oct 2022 03:34

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4X6

Tgt Ion: 43 Resp: 10237
 Ion Ratio Lower Upper
 43 100
 58 37.9 0.0 73.8

