

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051600.D
 Acq On : 29 Oct 2022 05:15
 Operator : JC/MD
 Sample : N5276-20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Y0

Quant Time: Oct 29 05:35:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Oct 29 00:39:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	176705	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	189267	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	75379	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	61564	4.626	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.600%
7) Chloroethane-d5	1.912	69	71137	5.125	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.600%
11) 1,1-Dichloroethene-d2	2.565	65	23021	4.766	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.400%
20) 2-Butanone-d5	4.617	46	271662	56.364	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.720%
24) Chloroform-d	5.060	84	160536	5.155	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
26) 1,2-Dichloroethane-d4	5.700	65	89372	5.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	5.726	84	282238	4.725	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
36) 1,2-Dichloropropane-d6	6.690	67	108046	5.173	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.400%
41) Toluene-d8	7.896	98	189591	4.037	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.800%
43) trans-1,3-Dichloroprop...	8.179	79	26025	4.075	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.600%
46) 2-Hexanone-d5	8.629	63	197303	51.325	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.640%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	102843	5.374	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.400%
66) 1,2-Dichlorobenzene-d4	12.192	152	74607	5.393	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds					Qvalue	
13) Acetone	2.623	43	11497	4.701	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051600.D
Acq On : 29 Oct 2022 05:15
Operator : JC/MD
Sample : N5276-20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4Y0

Quant Time: Oct 29 05:35:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Oct 29 00:39:42 2022
Response via : Initial Calibration

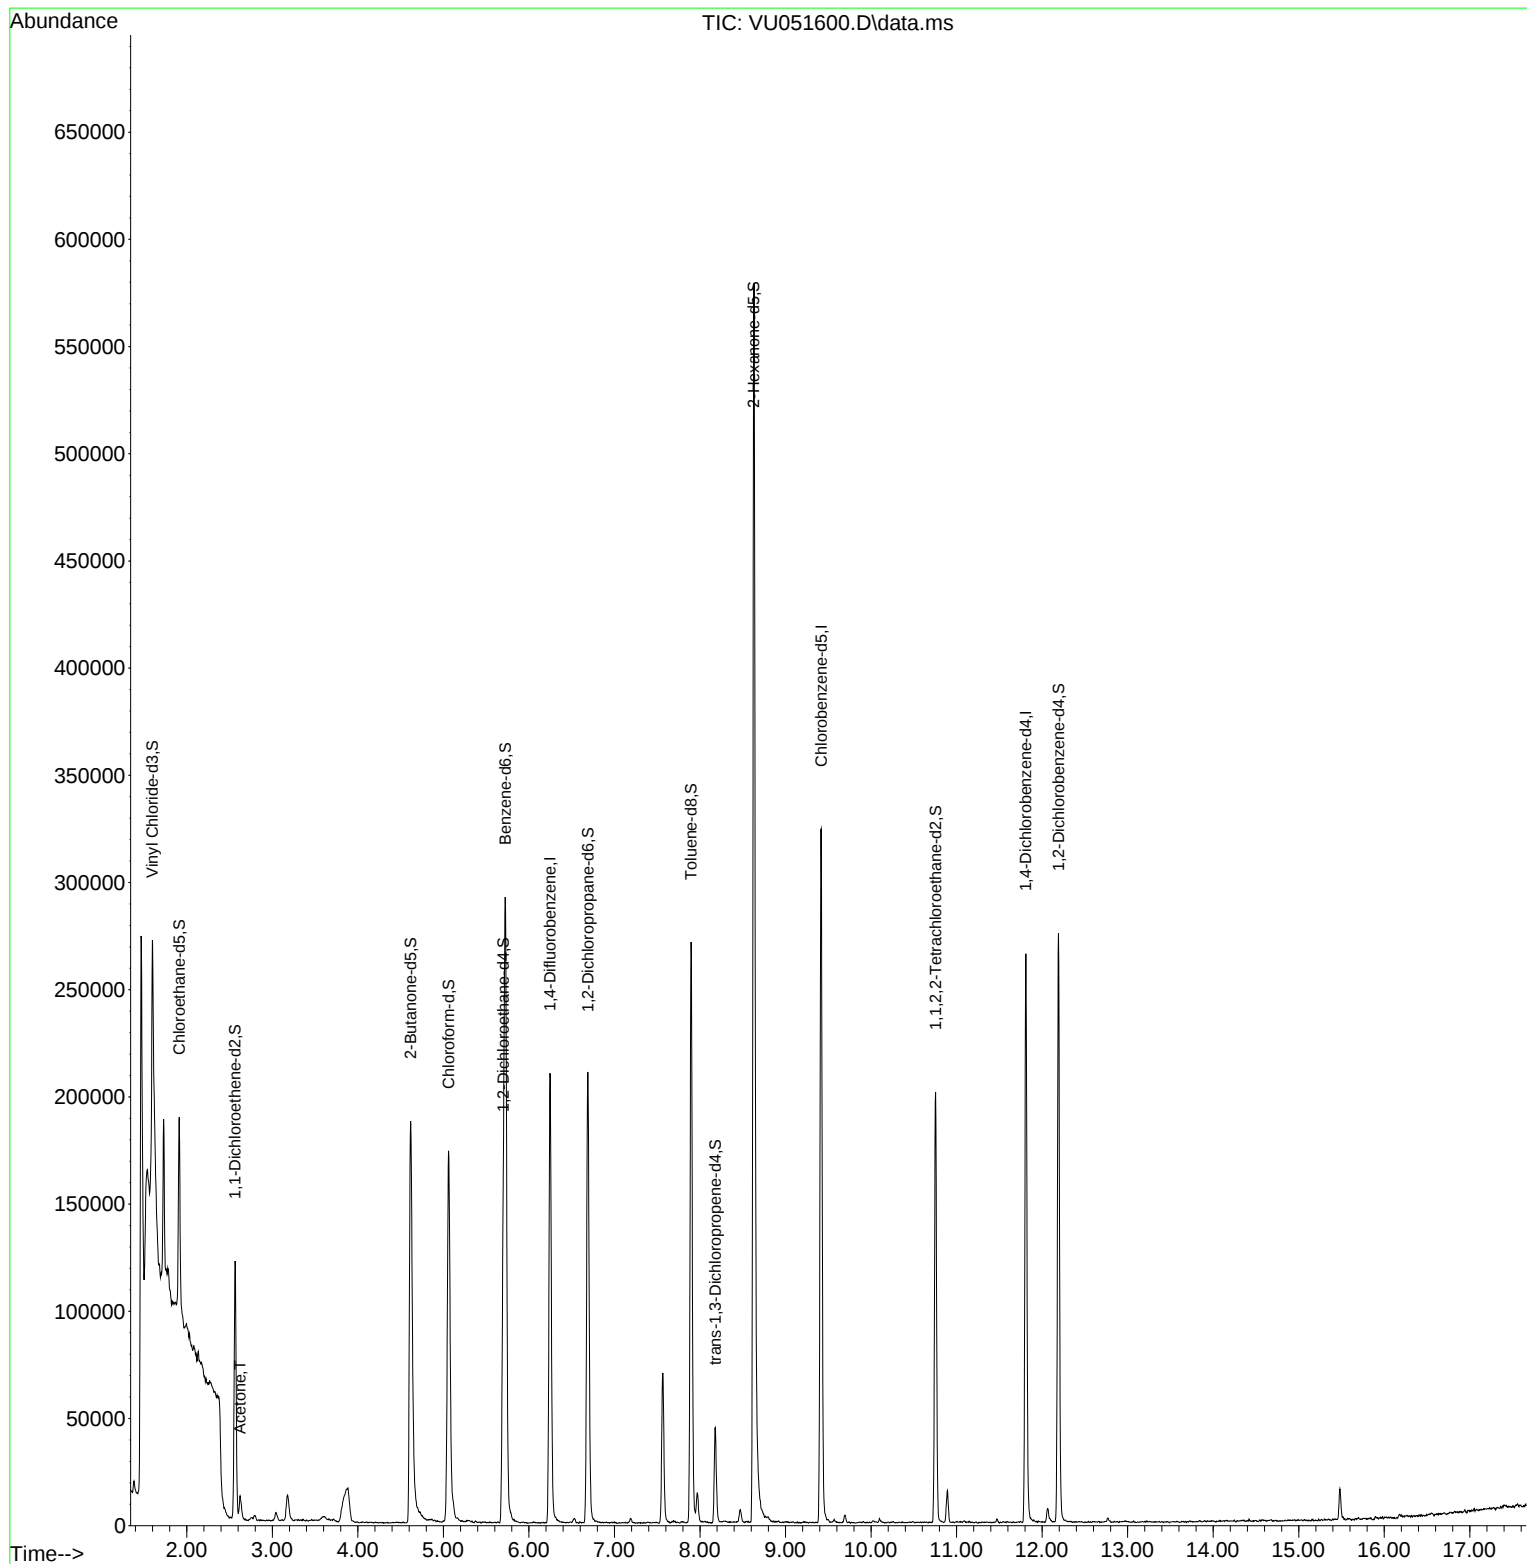

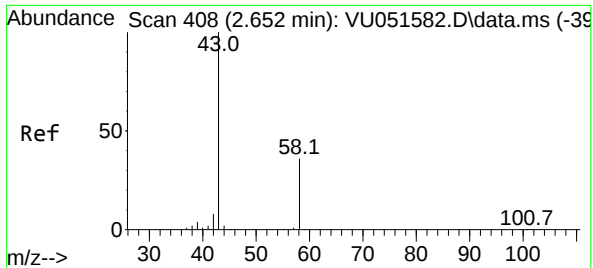

#13
 Acetone
 Concen: 4.701 ug/L
 RT: 2.623 min Scan# 31
 Delta R.T. -0.029 min
 Lab File: VU051600.D
 Acq: 29 Oct 2022 05:15

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4Y0

Tgt Ion: 43 Resp: 11497
 Ion Ratio Lower Upper
 43 100
 58 33.3 0.0 73.8

