

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051573.D
 Acq On : 28 Oct 2022 17:29
 Operator : JC/MD
 Sample : N5300-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHA88

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU051573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	52	80	87	rBV3	251444	783816	79.20%	9.533%
2	1.909	172	177	189	rVB	100014	131882	13.33%	1.604%
3	2.565	369	381	394	rBV	147861	237041	23.95%	2.883%
4	3.186	562	574	584	rBV2	6942	14494	1.46%	0.176%
5	3.867	758	786	802	rBV2	13631	47513	4.80%	0.578%
6	3.990	812	824	841	rVB3	8324	21005	2.12%	0.255%
7	4.620	1008	1020	1054	rBV	176357	449675	45.43%	5.469%
8	5.060	1139	1157	1181	rBV	173569	387745	39.18%	4.716%
9	5.723	1341	1363	1373	rBV2	322762	866037	87.50%	10.533%
10	5.771	1374	1378	1398	rVB	134461	242142	24.47%	2.945%
11	6.247	1512	1526	1544	rBV	268505	515812	52.12%	6.273%
12	6.690	1649	1664	1685	rBV	219375	431084	43.56%	5.243%
13	7.565	1924	1936	1951	rBV	70531	127965	12.93%	1.556%
14	7.896	2025	2039	2054	rBV	315216	551895	55.76%	6.712%
15	7.970	2054	2062	2075	rVB2	23134	41790	4.22%	0.508%
16	8.179	2113	2127	2145	rBV2	44059	77861	7.87%	0.947%
17	8.632	2255	2268	2301	rBV	522883	989722	100.00%	12.037%
18	9.417	2498	2512	2539	rBV2	400337	773622	78.17%	9.409%
19	9.571	2548	2560	2579	rVB	20802	37217	3.76%	0.453%
20	9.690	2586	2597	2611	rBV	42700	71020	7.18%	0.864%
21	10.102	2714	2725	2738	rVB2	15750	27360	2.76%	0.333%
22	10.755	2913	2928	2946	rBV	188685	301371	30.45%	3.665%
23	10.893	2960	2971	2986	rVB4	8442	15597	1.58%	0.190%
24	11.468	3141	3150	3159	rBV2	9467	13369	1.35%	0.163%
25	11.809	3244	3256	3276	rBV	339340	555863	56.16%	6.760%
26	12.192	3363	3375	3395	rBV	310969	509401	51.47%	6.195%




Sum of corrected areas: 8222299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051573.D
Acq On : 28 Oct 2022 17:29
Operator : JC/MD
Sample : N5300-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

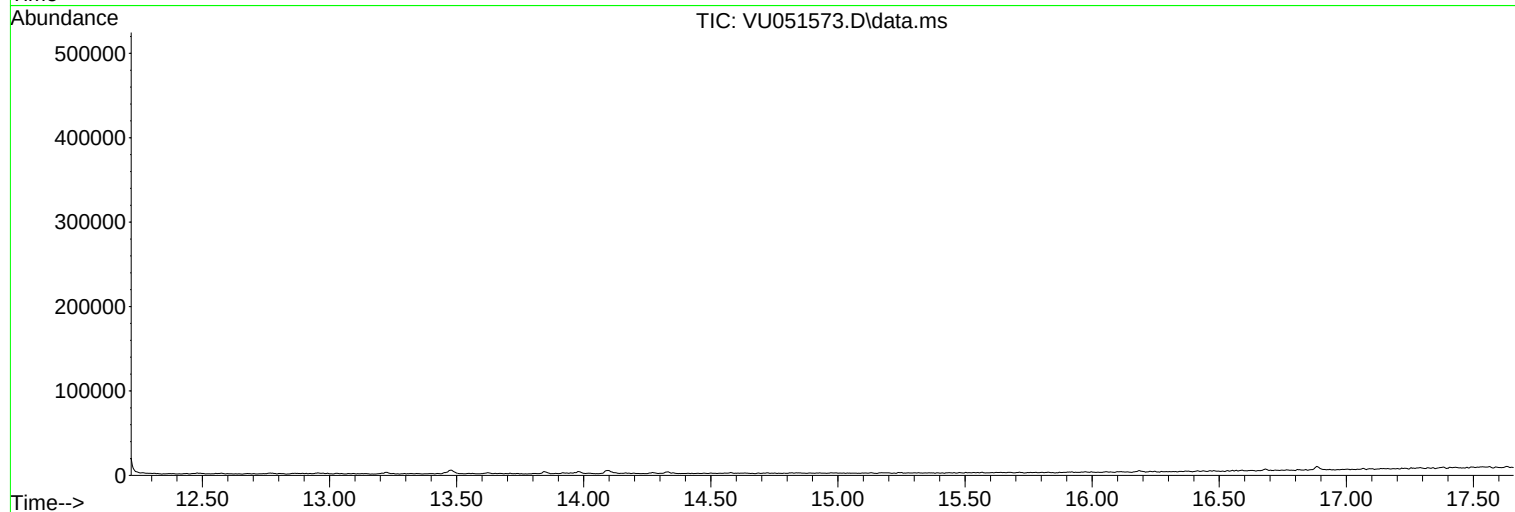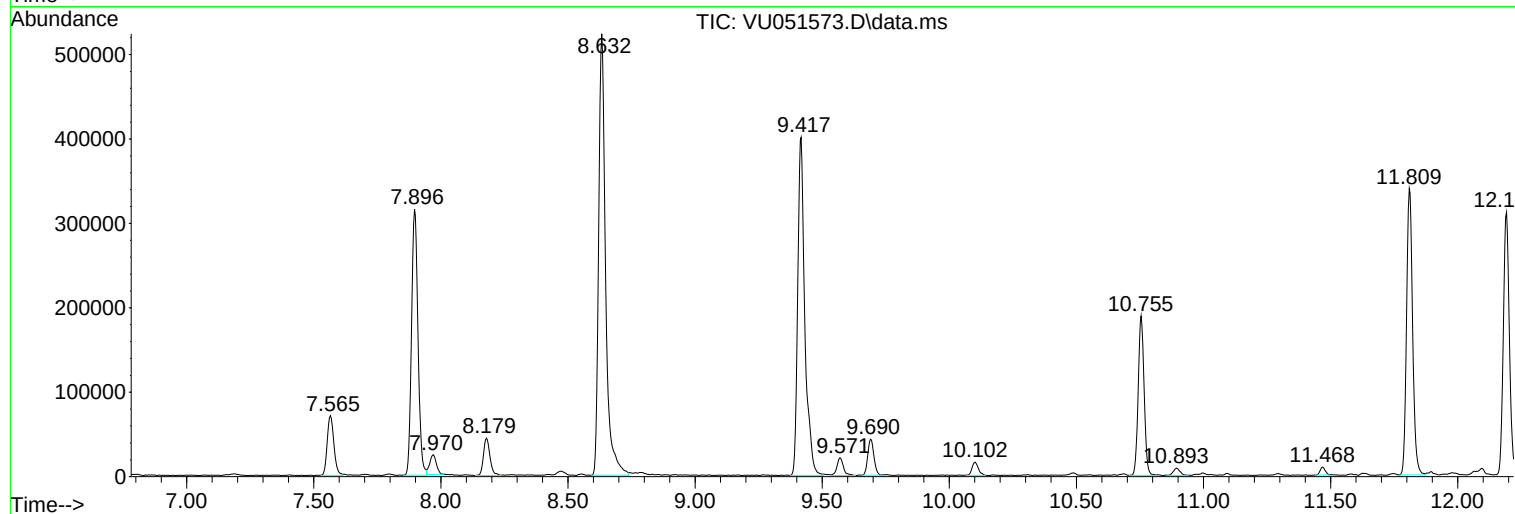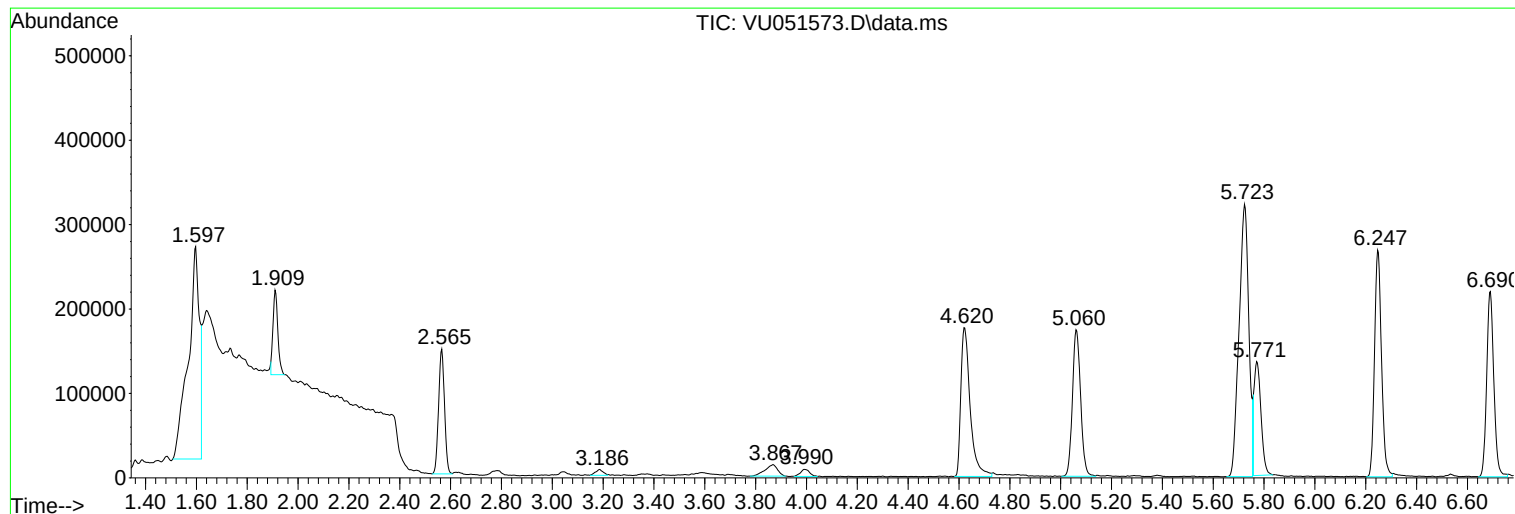

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051573.D
Acq On : 28 Oct 2022 17:29
Operator : JC/MD
Sample : N5300-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
Data File : VU051573.D
Acq On : 28 Oct 2022 17:29
Operator : JC/MD
Sample : N5300-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHA88

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
