
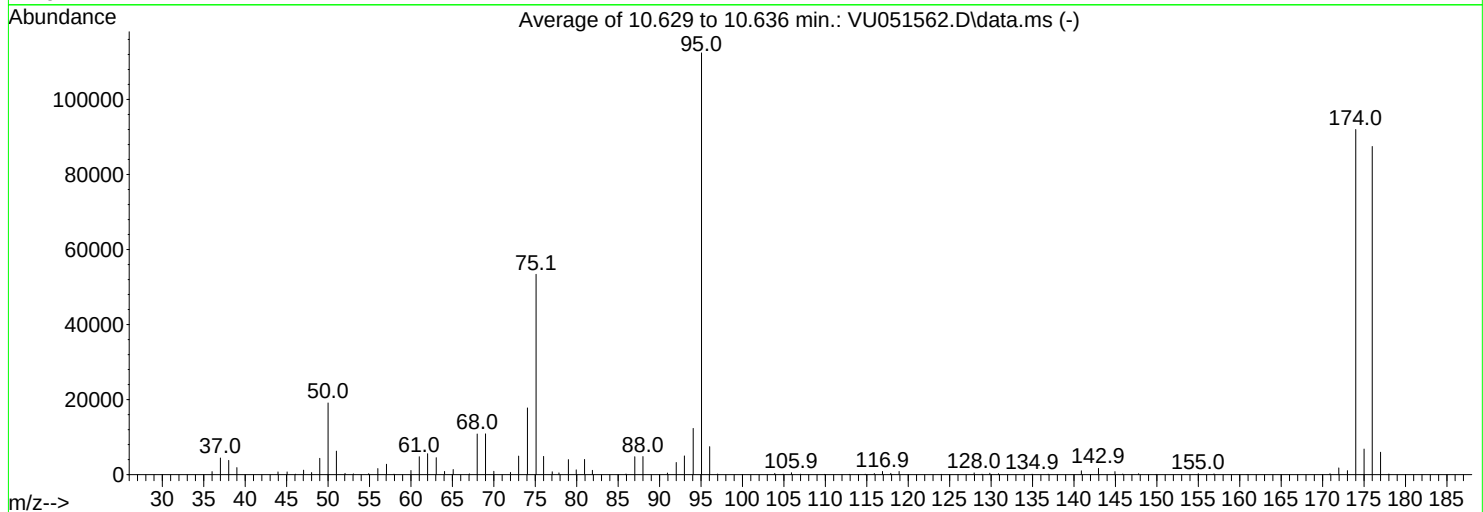


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102822\
 Data File : VU051562.D
 Acq On : 28 Oct 2022 10:19
 Operator : JC/MD
 Sample : BFB159
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB159

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 02 03:06:15 2022

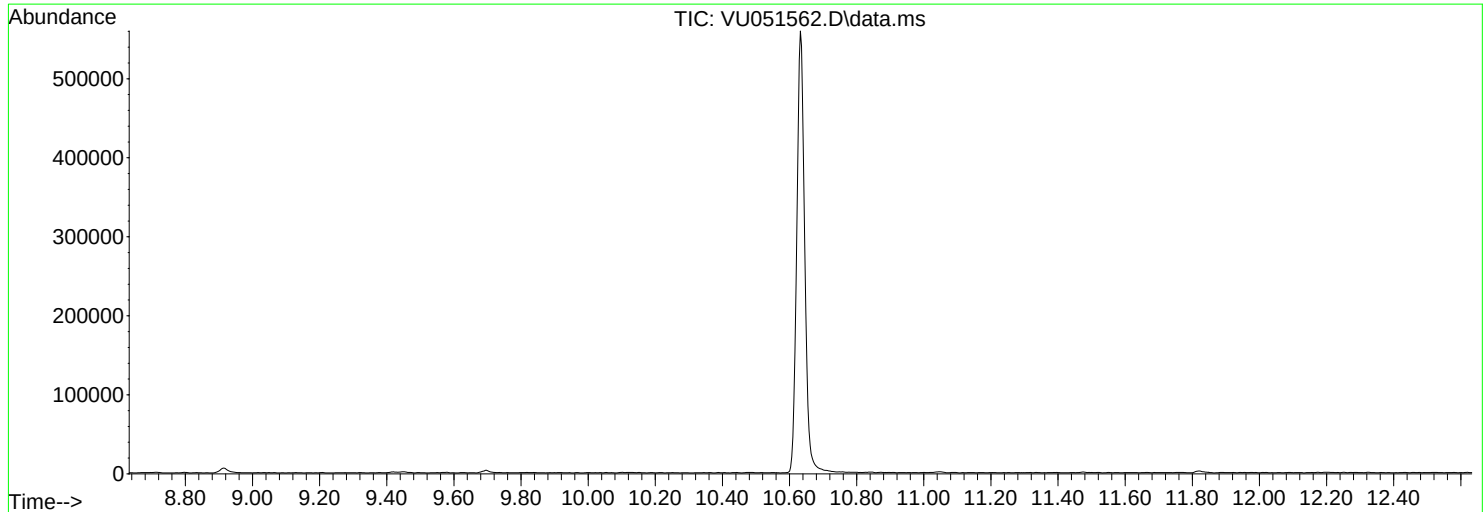

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	19131	PASS
75	95	30	80	47.5	53387	PASS
95	95	100	100	100.0	112424	PASS
96	95	5	9	6.6	7449	PASS
173	174	0.00	2	1.1	1050	PASS
174	95	50	120	81.8	92005	PASS
175	174	5	9	7.4	6839	PASS
176	174	95	101	95.1	87483	PASS
177	176	5	9	6.8	5979	PASS

m/z	Abundance
40.00	963.0
44.00	497.0

Instrument :
MSVOA_U
ClientSampleId :
BFB159

m/z	Abundance
36.00	765.0
37.00	4507.0
38.00	3901.0
39.00	1886.0
39.90	980.0
43.90	1270.0
45.00	716.0
46.10	162.0
47.10	1047.0
48.00	527.0
49.00	4277.0
50.00	18528.0
51.00	6096.0
52.00	353.0
53.00	138.0
54.90	295.0
56.00	1636.0
57.00	2789.0
58.00	138.0
60.00	1095.0
61.00	4713.0
62.00	5683.0
63.00	4367.0
64.10	867.0
65.10	1324.0
67.10	211.0
68.00	10685.0
69.00	11012.0
70.00	865.0
72.00	614.0
73.00	4775.0
74.00	16936.0
75.10	52648.0
76.00	4909.0
77.10	777.0
77.90	397.0
79.00	3975.0
79.90	1257.0
80.90	4008.0
81.90	1159.0
85.90	185.0
87.00	4598.0
88.00	4522.0
90.90	417.0
92.00	3131.0
93.00	4805.0
94.00	11706.0
95.10	109040.0
96.00	7376.0
97.00	213.0
103.90	365.0
104.80	109.0
105.90	459.0
107.00	151.0
114.80	168.0
115.90	298.0
116.90	789.0
117.90	367.0
118.90	832.0
124.00	143.0
127.90	496.0
128.90	146.0
129.80	409.0
130.90	283.0
134.90	103.0
136.90	117.0
140.90	891.0
142.00	104.0
142.90	1661.0
144.90	757.0
145.90	141.0
147.80	206.0
149.90	153.0
155.00	281.0
156.90	198.0
170.90	280.0
171.90	1676.0
173.00	1038.0
174.00	87552.0
175.00	6679.0
176.00	82296.0
177.00	6127.0
178.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB159

m/z	Abundance
36.00	846.0
37.00	4577.0
38.00	3855.0
39.00	1890.0
39.90	919.0
43.90	1256.0
45.00	769.0
46.00	129.0
47.00	1251.0
48.00	554.0
49.00	4551.0
50.00	19824.0
51.00	6543.0
52.10	360.0
53.10	265.0
54.90	270.0
56.00	1710.0
57.10	2886.0
57.90	117.0
60.00	1141.0
61.00	4886.0
62.00	5888.0
63.10	4628.0
64.00	871.0
65.10	1417.0
67.10	231.0
68.00	11160.0
69.00	11214.0
70.00	912.0
72.00	646.0
73.00	5164.0
74.10	18464.0
75.10	55240.0
76.00	5084.0
77.10	780.0
77.80	491.0
79.00	4163.0
79.90	1347.0
81.00	4198.0
81.90	1223.0
86.00	172.0
87.00	4899.0
88.00	4846.0
91.00	427.0
92.00	3405.0
93.00	5117.0
94.10	12727.0
95.10	116176.0
96.10	7733.0
97.00	197.0
103.90	370.0
104.90	127.0
105.90	535.0
107.00	136.0
109.90	102.0
112.90	109.0
114.80	148.0
115.90	281.0
116.90	844.0
117.90	354.0
118.90	883.0
124.00	145.0
128.00	528.0
128.90	145.0
129.80	399.0
130.90	296.0
134.90	117.0
136.90	130.0
140.90	1056.0
142.90	1695.0
144.90	862.0
145.90	155.0
147.80	265.0
149.90	147.0
155.00	257.0
156.90	231.0
170.90	268.0
172.00	1849.0
173.00	1114.0
174.00	95328.0
175.00	7065.0
176.00	90680.0
177.00	6145.0
178.00	210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB159

m/z	Abundance
36.00	812.0
37.00	4258.0
38.00	3683.0
39.00	1883.0
39.90	878.0
44.00	1176.0
45.10	746.0
46.00	153.0
47.00	1337.0
48.00	558.0
49.00	4268.0
50.00	19040.0
51.00	6148.0
52.00	320.0
53.10	303.0
54.90	245.0
56.00	1533.0
57.10	2692.0
57.90	101.0
60.00	1107.0
61.00	4792.0
62.00	5260.0
63.10	4581.0
64.00	864.0
65.10	1354.0
67.00	219.0
68.00	10706.0
69.00	10402.0
70.00	854.0
72.00	587.0
73.00	4951.0
74.10	17952.0
75.10	52272.0
76.00	4580.0
77.00	742.0
77.80	526.0
79.00	3937.0
80.00	1287.0
81.00	3984.0
81.90	1066.0
86.00	122.0
87.00	4813.0
88.00	5057.0
91.00	407.0
92.00	3233.0
93.00	5077.0
94.10	12500.0
95.00	112056.0
96.10	7238.0
97.00	163.0
103.90	347.0
105.00	144.0
105.90	566.0
107.00	115.0
109.90	105.0
112.90	102.0
114.80	104.0
115.90	312.0
116.90	884.0
117.90	347.0
118.90	800.0
127.90	442.0
128.90	111.0
129.90	380.0
130.90	222.0
135.00	143.0
136.90	148.0
140.90	1123.0
143.00	1650.0
145.00	856.0
145.90	177.0
147.80	266.0
155.00	224.0
156.90	255.0
160.90	121.0
170.90	208.0
172.00	1837.0
173.00	998.0
174.00	93136.0
175.00	6772.0
176.00	89472.0
177.00	5666.0
178.00	223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB159