




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
 Data File : VU055974.D
 Acq On : 28 Oct 2023 15:16
 Operator : MD/SY
 Sample : 05114-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B58

Manual IntegrationsAPPROVED

Quant Time: Oct 30 04:54:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 04:51:15 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 11/01/2023

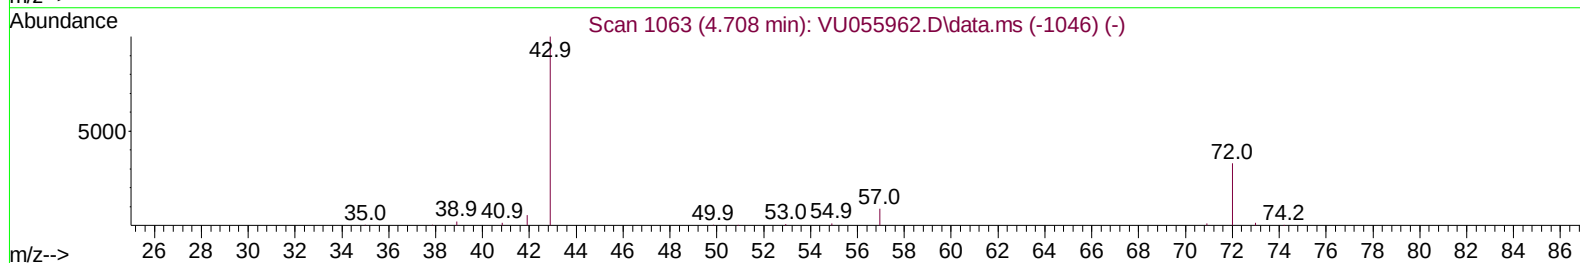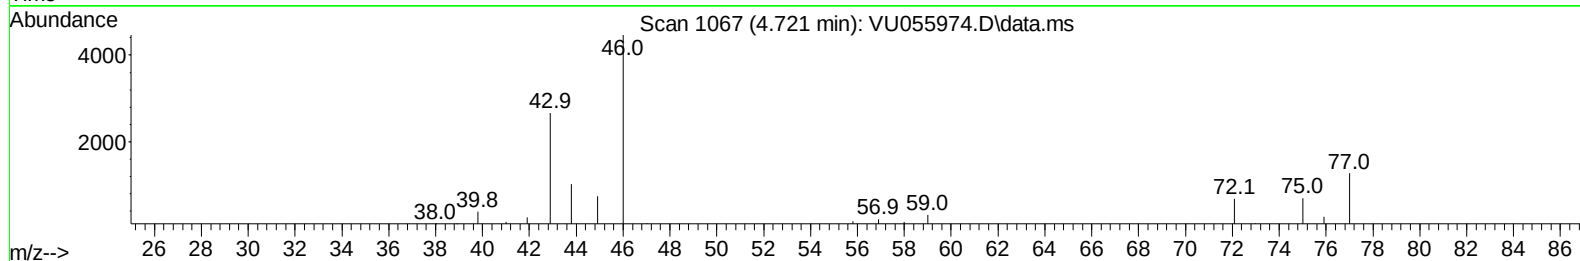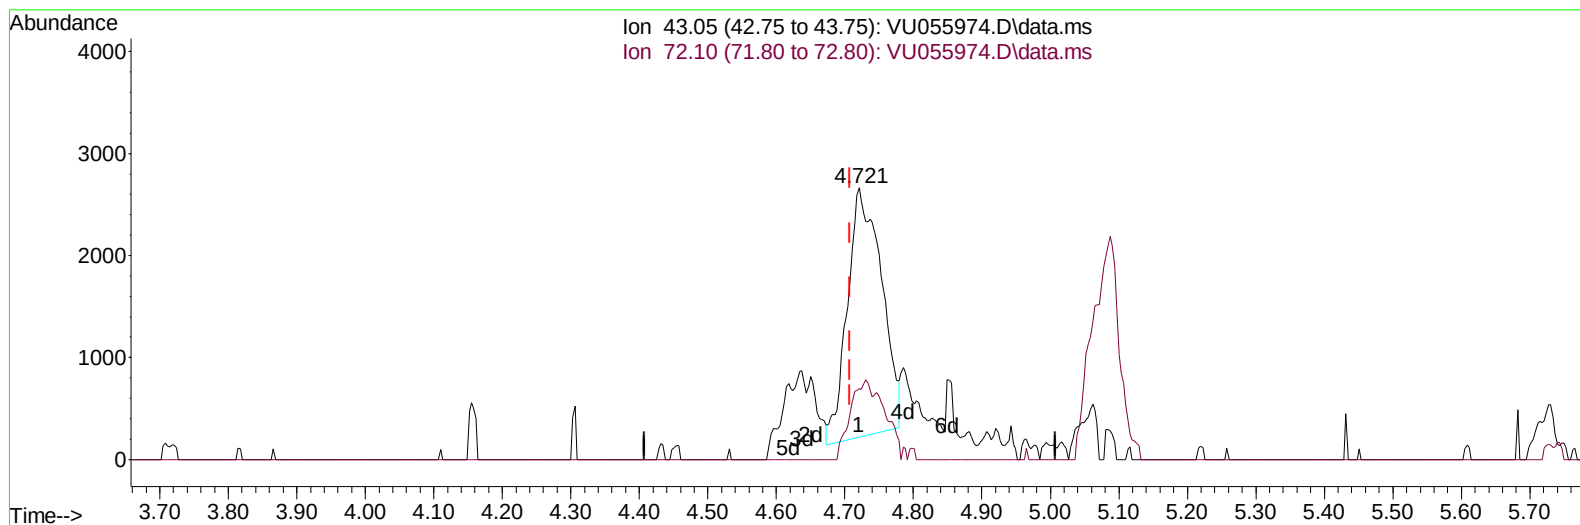

TIC: VU055974.D\data.ms

(21) 2-Butanone (T)

4.721min (+ 0.013) 2.06 ug/L

response 8406

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.90	19.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
 Data File : VU055974.D
 Acq On : 28 Oct 2023 15:16
 Operator : MD/SY
 Sample : 05114-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B58

Manual IntegrationsAPPROVED

Quant Time: Oct 30 04:54:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 04:51:15 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 11/01/2023

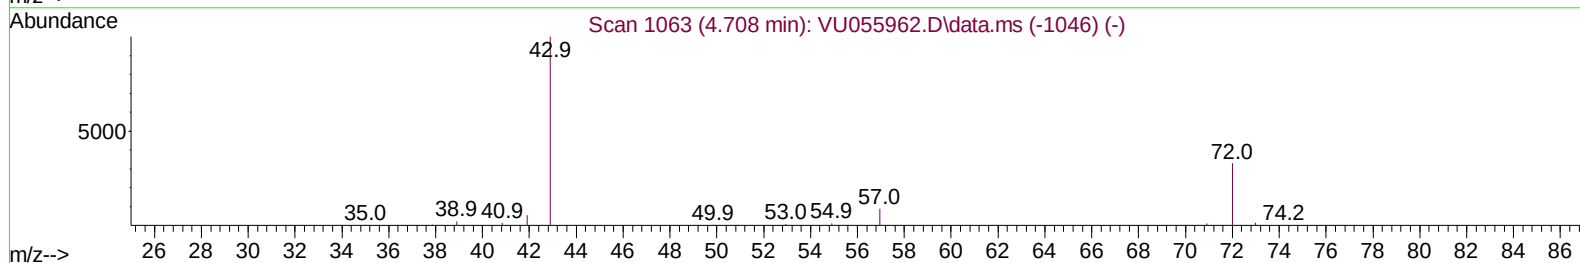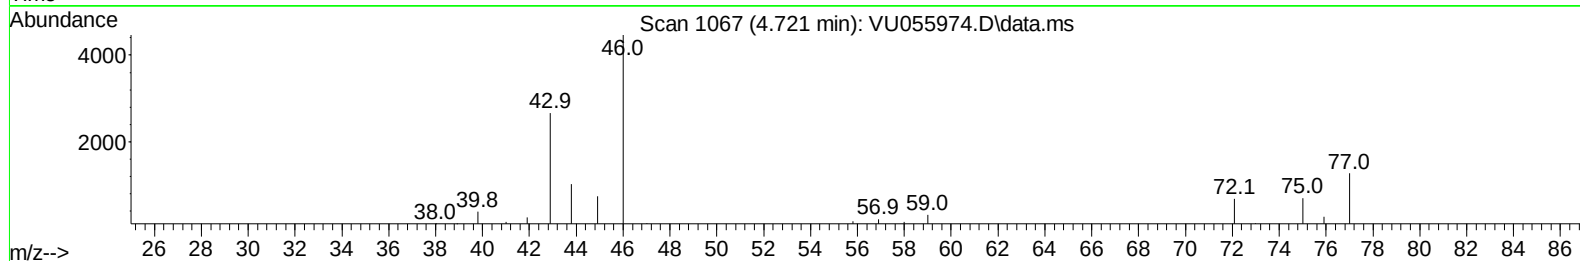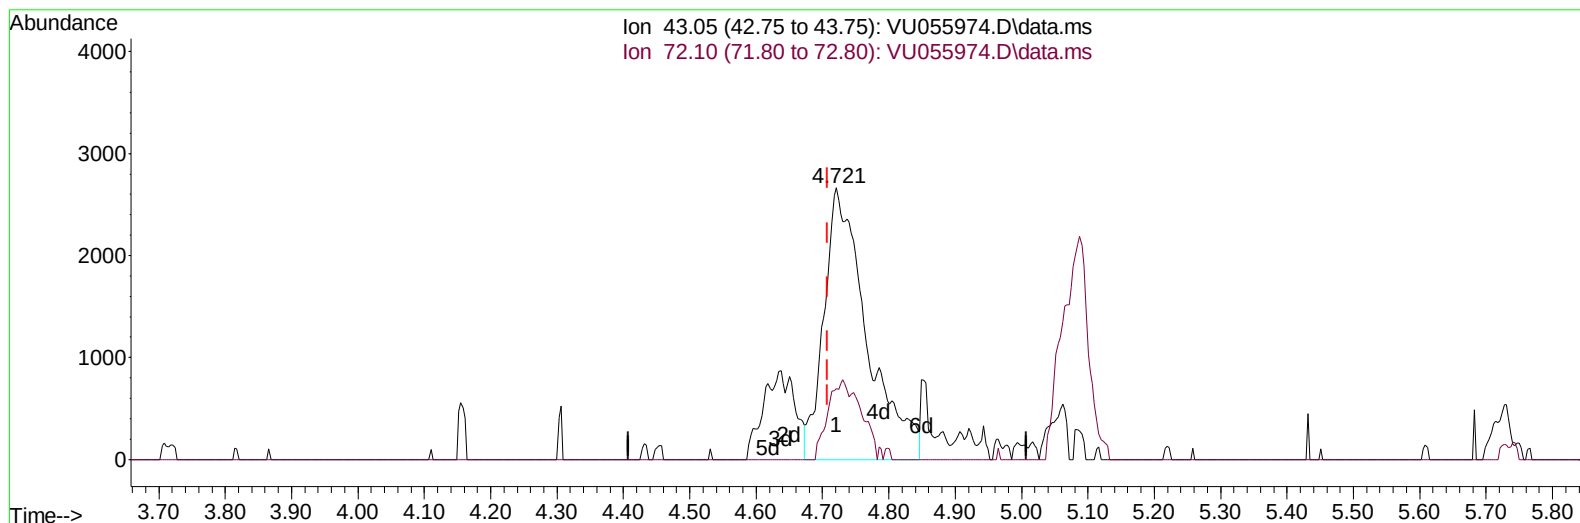

TIC: VU055974.D\data.ms

(21) 2-Butanone (T)

4.721min (+ 0.013) 2.92 ug/L m

response 11927

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	28.90	13.88#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
 Data File : VU055974.D
 Acq On : 28 Oct 2023 15:16
 Operator : MD/SY
 Sample : 05114-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B58

Manual IntegrationsAPPROVED

Quant Time: Oct 30 04:54:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Oct 30 04:51:15 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
 Supervised By :Mahesh Dadoda 11/01/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.248	114	345358	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	344287	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	160856	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	119817	4.386	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	87.800%	
7) Chloroethane-d5	1.914	69	106920	5.021	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	100.400%	
11) 1,1-Dichloroethene-d2	2.567	65	54829	4.727	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	94.600%	
20) 2-Butanone-d5	4.624	46	265736	54.524	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	109.040%	
24) Chloroform-d	5.062	84	286634	5.662	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	113.200%	
26) 1,2-Dichloroethane-d4	5.698	65	123853	5.022	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	100.400%	
32) Benzene-d6	5.724	84	529616	5.164	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	103.200%	
36) 1,2-Dichloropropane-d6	6.689	67	162582	5.348	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	107.000%	
41) Toluene-d8	7.894	98	462958	4.976	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.600%	
43) trans-1,3-Dichloroprop...	8.177	79	56173	4.724	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	94.400%	
46) 2-Hexanone-d5	8.631	63	211614	70.108	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	140.220%#	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	116918	5.281	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	105.600%	
66) 1,2-Dichlorobenzene-d4	12.190	152	166174	5.537	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	110.800%	
Target Compounds						
					Qvalue	
13) Acetone	2.641	43	14048	5.058	ug/L	98
21) 2-Butanone	4.721	43	11927m	2.921	ug/L	
25) Chloroform	5.084	83	663566	18.365	ug/L	99
38) Bromodichloromethane	7.103	83	113786	4.493	ug/L	99
49) Dibromochloromethane	8.808	129	18839	1.210	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
Data File : VU055974.D
Acq On : 28 Oct 2023 15:16
Operator : MD/SY
Sample : 05114-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B58

Manual IntegrationsAPPROVED

Quant Time: Oct 30 04:54:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Oct 30 04:51:15 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/30/2023
Supervised By :Mahesh Dadoda 11/01/2023

