

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
 Data File : VU055963.D
 Acq On : 28 Oct 2023 10:41
 Operator : MD/SY
 Sample : VU1028WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK056

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	108	rBV	133255	151480	13.54%	1.649%
2	1.914	185	194	214	rVB	107679	149488	13.36%	1.627%
3	2.567	382	397	415	rBV	240404	397877	35.56%	4.331%
4	3.046	534	546	562	rBV5	7928	17035	1.52%	0.185%
5	3.184	574	589	605	rBV2	11041	24817	2.22%	0.270%
6	4.631	1020	1039	1070	rBV3	120163	379780	33.94%	4.134%
7	5.059	1156	1172	1207	rVB2	211582	486033	43.44%	5.291%
8	5.724	1358	1379	1413	rBV2	429406	1118964	100.00%	12.180%
9	6.245	1526	1541	1572	rBV	392840	781659	69.86%	8.509%
10	6.689	1663	1679	1703	rBV	249059	509687	45.55%	5.548%
11	7.563	1935	1951	1979	rBV	114376	217866	19.47%	2.372%
12	7.895	2041	2054	2076	rBV	514960	945472	84.50%	10.292%
13	8.181	2132	2143	2161	rBV2	65953	124856	11.16%	1.359%
14	8.634	2271	2284	2326	rBV2	421800	965238	86.26%	10.507%
15	9.415	2514	2527	2550	rBV	548795	965325	86.27%	10.508%
16	10.753	2930	2943	2962	rBV	175377	287773	25.72%	3.132%
17	11.811	3259	3272	3293	rBV	520845	876793	78.36%	9.544%
18	12.190	3375	3390	3416	rBV	444728	761342	68.04%	8.287%
19	13.853	3899	3907	3917	rBV4	7748	12334	1.10%	0.134%
20	14.338	4044	4058	4068	rBV6	6413	12921	1.15%	0.141%




Sum of corrected areas: 9186740

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
Data File : VU055963.D
Acq On : 28 Oct 2023 10:41
Operator : MD/SY
Sample : VU1028WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK056

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

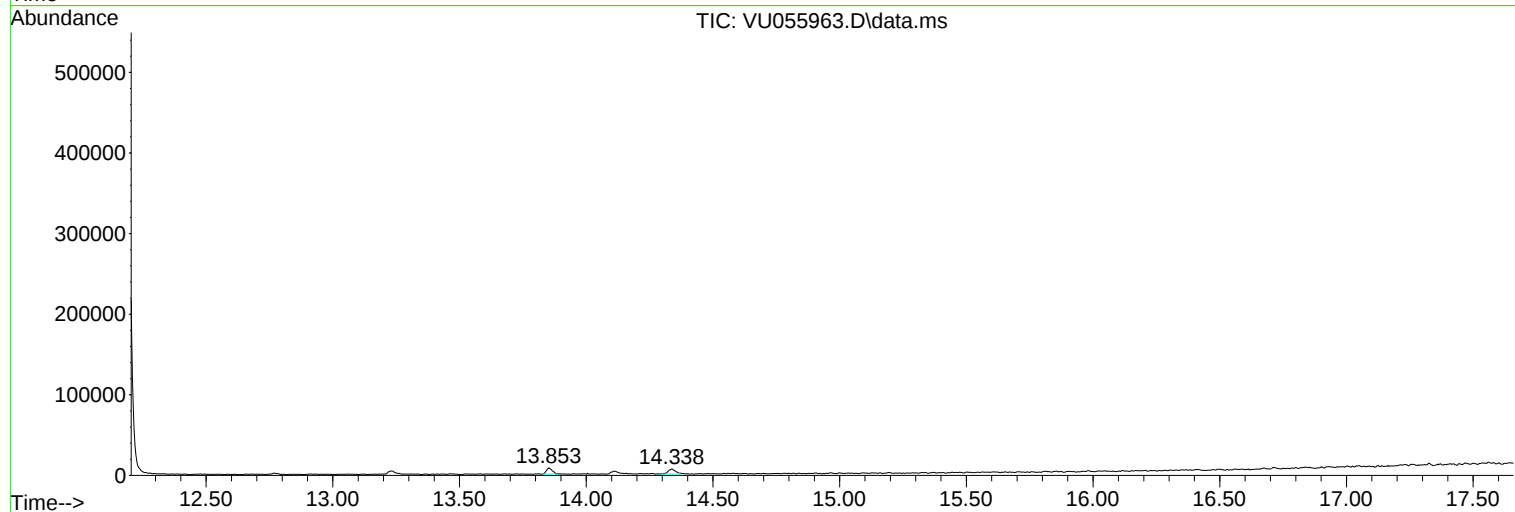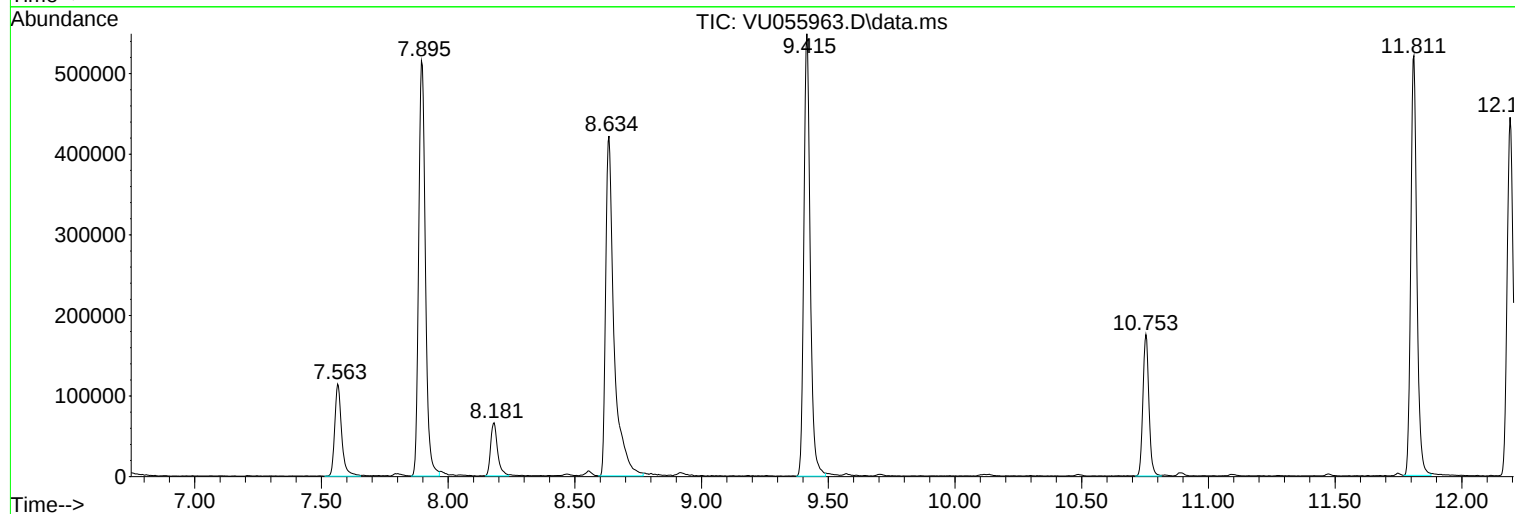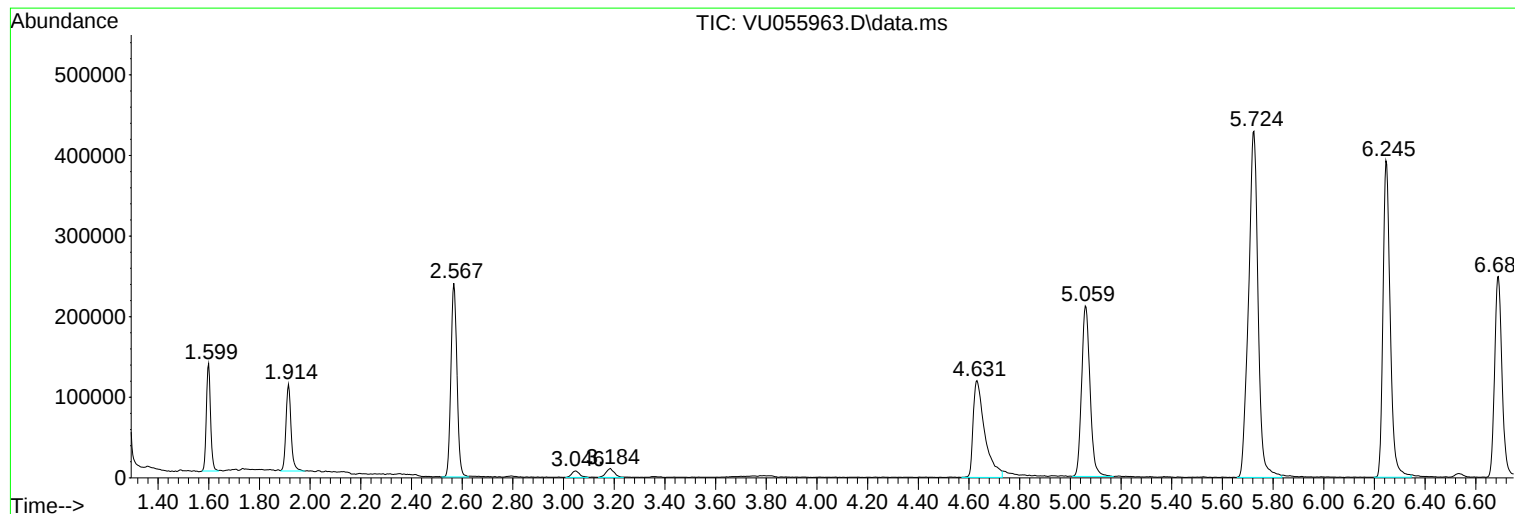

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
Data File : VU055963.D
Acq On : 28 Oct 2023 10:41
Operator : MD/SY
Sample : VU1028WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK056

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
Data File : VU055963.D
Acq On : 28 Oct 2023 10:41
Operator : MD/SY
Sample : VU1028WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK056

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc