

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
 Data File : VU055976.D
 Acq On : 28 Oct 2023 16:05
 Operator : MD/SY
 Sample : 05114-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B60

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.489	56	62	77	rBV	49957	51160	2.46%	0.409%
2	1.599	88	96	111	rVB	153357	177431	8.52%	1.418%
3	1.914	186	194	209	rVB	126286	171563	8.24%	1.371%
4	2.566	384	397	410	rBV	267862	441787	21.23%	3.531%
5	3.190	574	591	618	rBV2	25930	94266	4.53%	0.753%
6	4.627	1019	1038	1083	rBV3	163702	511420	24.57%	4.088%
7	5.081	1157	1179	1205	rBV3	758523	2081411	100.00%	16.636%
8	5.724	1357	1379	1410	rBV2	495006	1286289	61.80%	10.281%
9	6.248	1528	1542	1570	rBV	398227	793138	38.11%	6.339%
10	6.688	1661	1679	1703	rBV	295885	593169	28.50%	4.741%
11	7.103	1795	1808	1831	rBV	162898	311606	14.97%	2.490%
12	7.563	1939	1951	1973	rBV	135643	255623	12.28%	2.043%
13	7.894	2040	2054	2073	rBV	604166	1095260	52.62%	8.754%
14	8.177	2131	2142	2158	rBV	81201	146749	7.05%	1.173%
15	8.634	2271	2284	2325	rBV2	533237	1204233	57.86%	9.625%
16	8.807	2328	2338	2351	rVB2	35098	65181	3.13%	0.521%
17	9.415	2513	2527	2551	rBV	566580	993291	47.72%	7.939%
18	10.753	2928	2943	2965	rBV	210867	352266	16.92%	2.815%
19	11.810	3259	3272	3296	rBV	556962	939272	45.13%	7.507%
20	12.190	3376	3390	3418	rBV	553342	946679	45.48%	7.566%




Sum of corrected areas: 12511794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
Data File : VU055976.D
Acq On : 28 Oct 2023 16:05
Operator : MD/SY
Sample : 05114-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

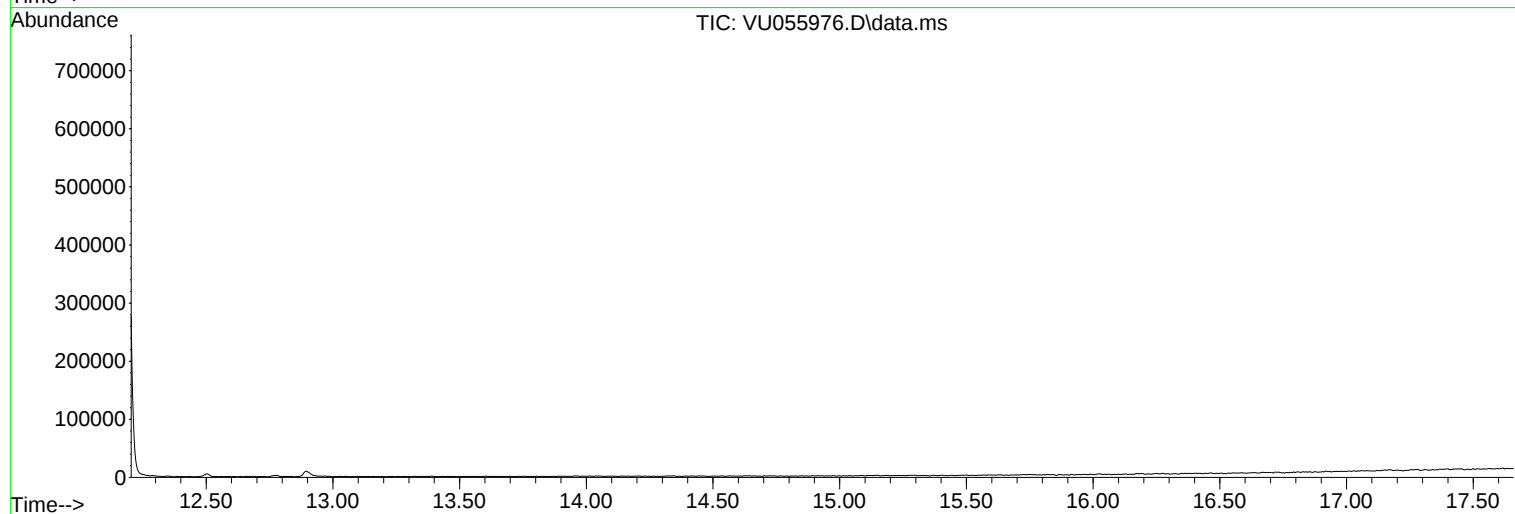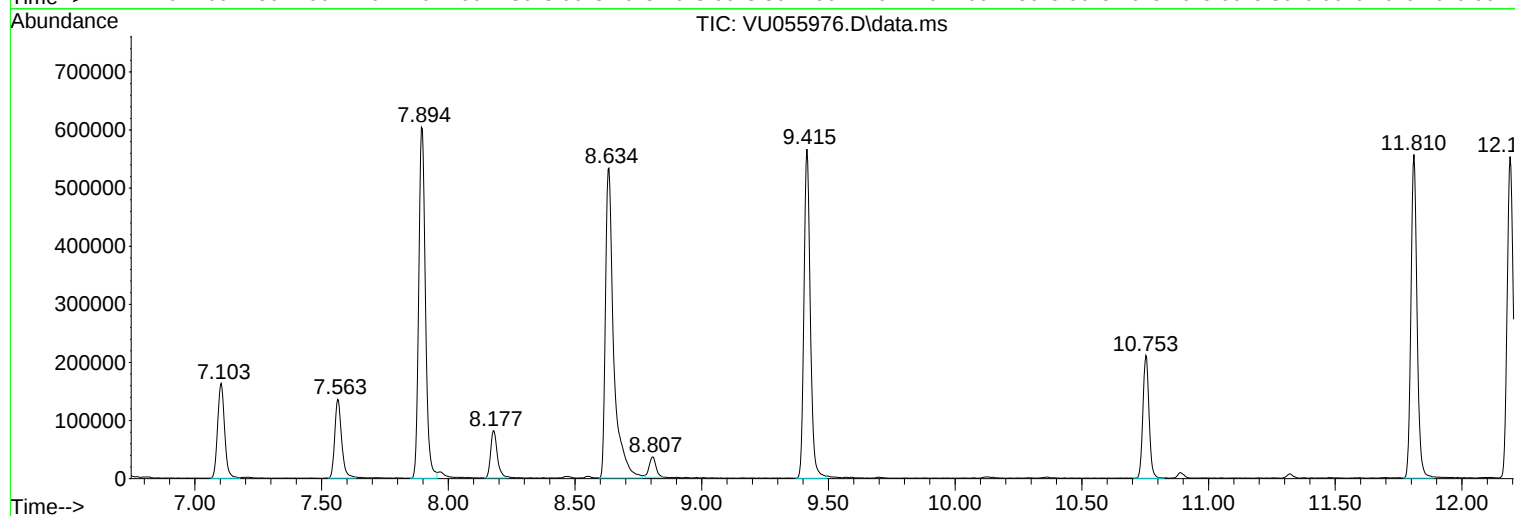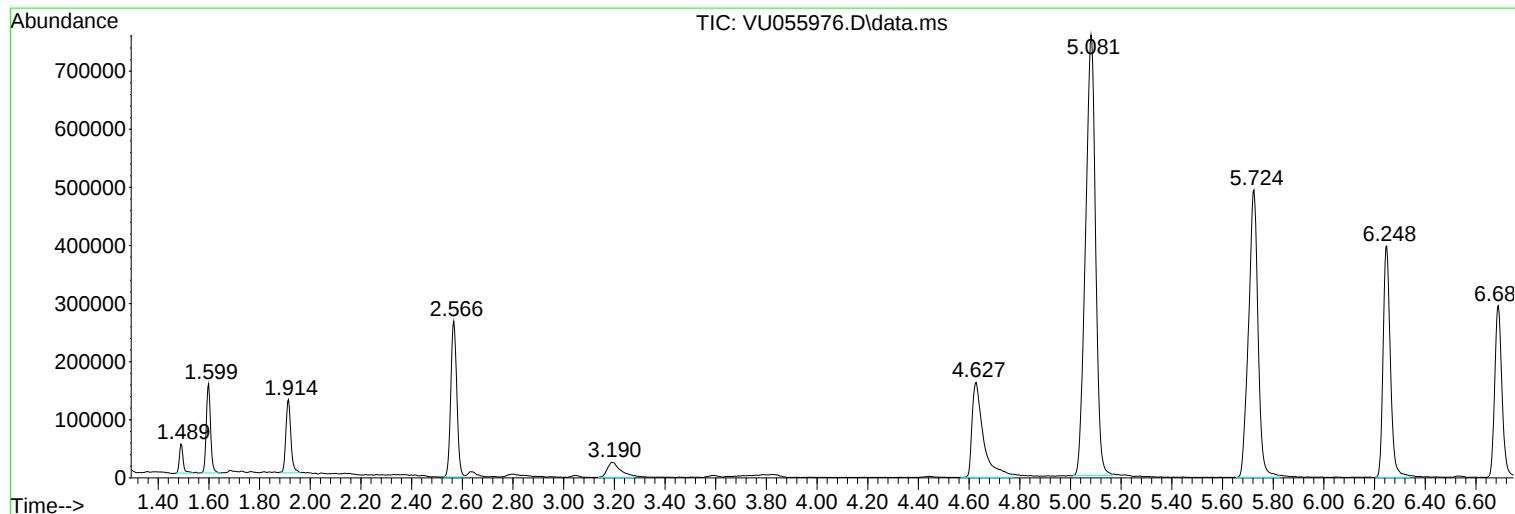

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
Data File : VU055976.D
Acq On : 28 Oct 2023 16:05
Operator : MD/SY
Sample : 05114-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B60










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Butanol, 3-methoxy- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.190	0.59 ug/L	94266	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Butanol, 3-methoxy-			104	C5H12O2	002517-43-3	72
2	1-Butanol, 3-methoxy-			104	C5H12O2	002517-43-3	40
3	3-Pentanol			88	C5H12O	000584-02-1	33
4	1,2-Butanediol			90	C4H10O2	000584-03-2	33
5	1,2-Butanediol			90	C4H10O2	000584-03-2	28

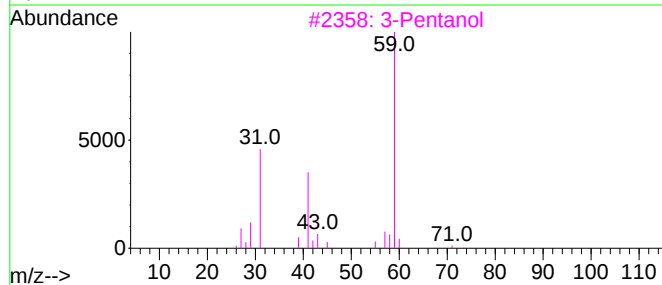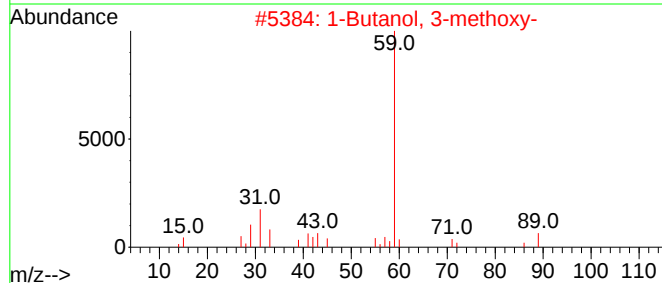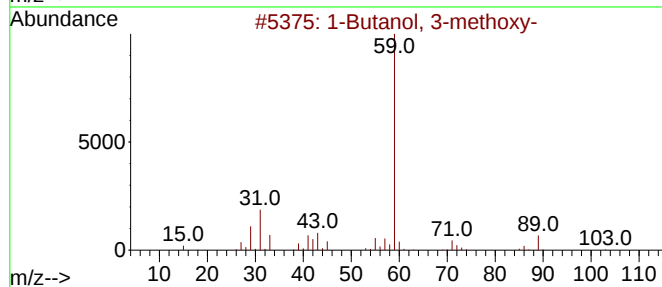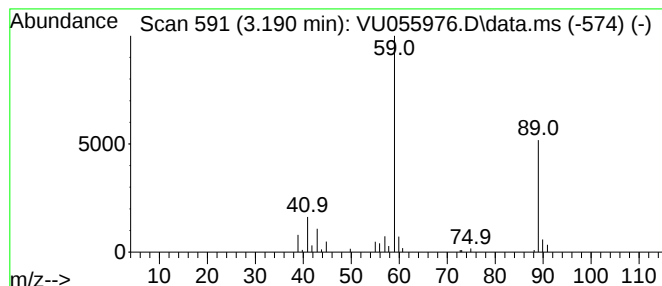

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102823\
Data File : VU055976.D
Acq On : 28 Oct 2023 16:05
Operator : MD/SY
Sample : 05114-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Butanol, 3-me...	3.190	0.6	ug/L	94266	1	6.248	793138	5.0