

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\U102918\
 Data File : VU027853.D
 Acq On : 29 Oct 2018 14:08
 Operator : MD/SY
 Sample : J5716-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBY1

Quant Time: Oct 30 03:04:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 02:27:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	114538	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	106853	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	49819	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	32267	36.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	72.42%
7) Chloroethane-d5	1.68	69	25977	37.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.72%
11) 1,1-Dichloroethene-d2	2.28	63	46886	29.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.42%#
21) 2-Butanone-d5	4.18	46	62430	82.20	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.20%
24) Chloroform-d	4.65	84	62401	38.95	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.90%
26) 1,2-Dichloroethane-d4	5.31	65	45377	40.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.80%
32) Benzene-d6	5.34	84	123779	40.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.36%
36) 1,2-Dichloropropane-d6	6.33	67	44356	40.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	81.66%
41) Toluene-d8	7.57	98	115572	41.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.34%
43) trans-1,3-Dichloropropene-	7.85	79	21122	40.04	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.08%
47) 2-Hexanone-d5	8.31	63	47455	85.36	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.36%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	58138	41.44	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.88%
64) 1,2-Dichlorobenzene-d4	11.86	152	42324	41.48	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.96%


Target Compounds					Qvalue
13) Acetone	2.32	43	3482	6.58 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102918\
Data File : VU027853.D
Acq On : 29 Oct 2018 14:08
Operator : MD/SY
Sample : J5716-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBY1

Quant Time: Oct 30 03:04:50 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 02:27:31 2018
Response via : Initial Calibration

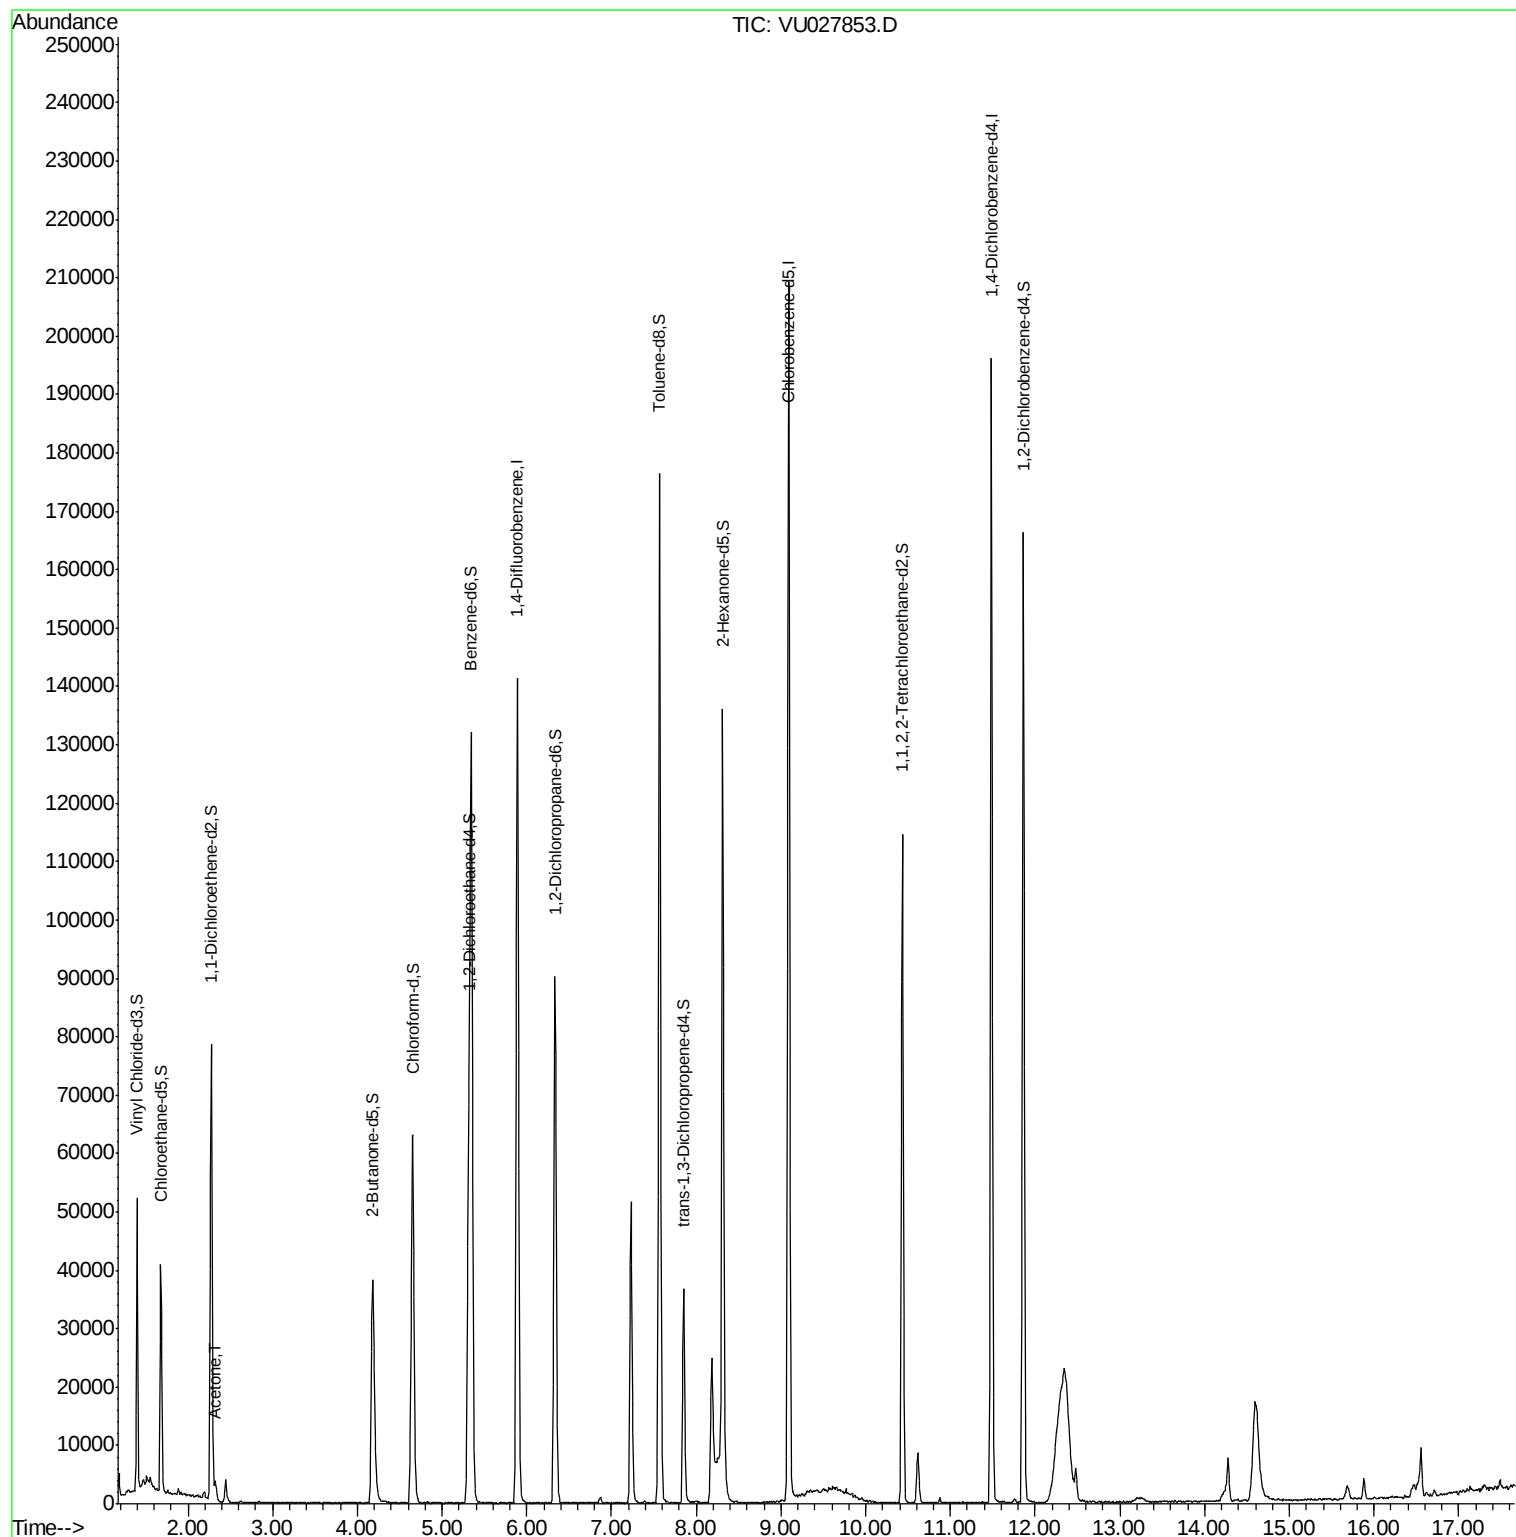

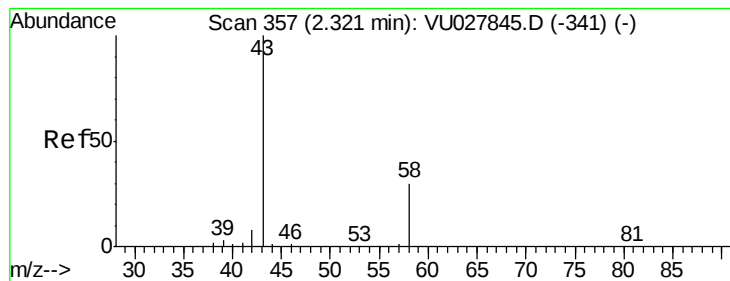

#13
 Acetone
 Concen: 6.58 ug/L
 RT: 2.32 min Scan# 357
 Delta R.T. 0.00 min
 Lab File: VU027853.D
 Acq: 29 Oct 2018 14:08

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBY1

Tgt Ion: 43 Resp: 3482
 Ion Ratio Lower Upper
 43 100
 58 25.6 0.0 57.4

