

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102918\
 Data File : VU027856.D
 Acq On : 29 Oct 2018 15:17
 Operator : MD/SY
 Sample : J5716-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBS9

Quant Time: Oct 30 03:49:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 02:27:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	109706	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	103628	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	49230	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	31900	37.37	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.74%
7) Chloroethane-d5	1.68	69	26043	39.63	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.26%
11) 1,1-Dichloroethene-d2	2.27	63	46157	30.02	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.04%
21) 2-Butanone-d5	4.18	46	64100	88.12	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.12%
24) Chloroform-d	4.65	84	61390	40.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.02%
26) 1,2-Dichloroethane-d4	5.31	65	44675	42.04	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.08%
32) Benzene-d6	5.34	84	122139	41.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.78%
36) 1,2-Dichloropropane-d6	6.33	67	44492	42.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.46%
41) Toluene-d8	7.57	98	113361	41.64	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.28%
43) trans-1,3-Dichloropropene-	7.85	79	20725	40.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.02%
47) 2-Hexanone-d5	8.31	63	47076	87.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.31%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	56835	41.77	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.54%
64) 1,2-Dichlorobenzene-d4	11.86	152	43410	43.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.10%


Target Compounds					Qvalue
13) Acetone	2.32	43	3689	7.28 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102918\
Data File : VU027856.D
Acq On : 29 Oct 2018 15:17
Operator : MD/SY
Sample : J5716-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBS9

Quant Time: Oct 30 03:49:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 02:27:31 2018
Response via : Initial Calibration

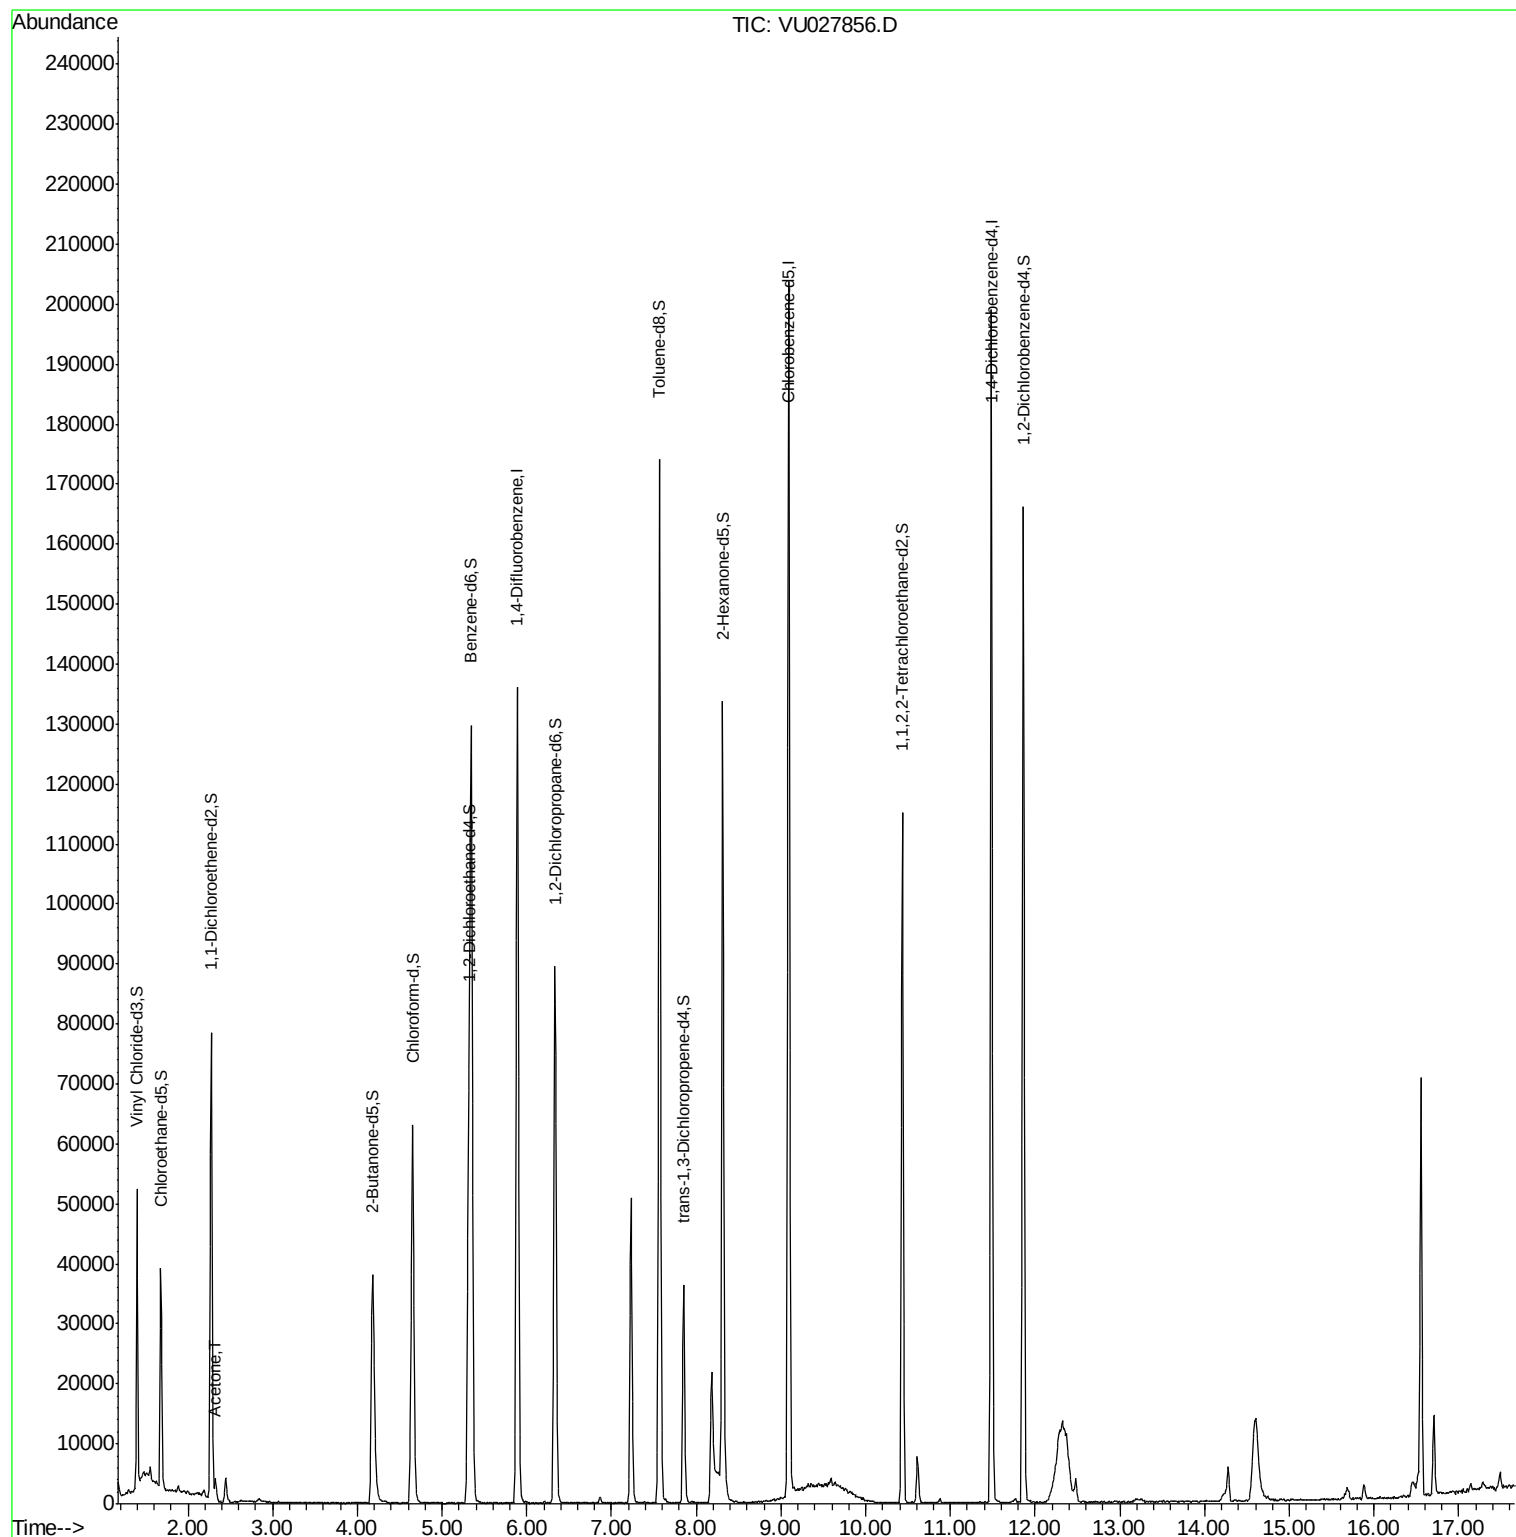

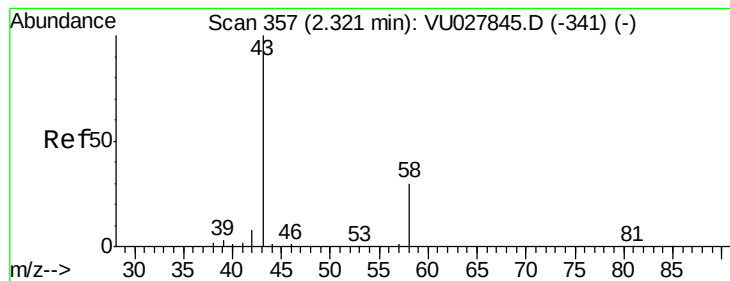

#13
 Acetone
 Concen: 7.28 ug/L
 RT: 2.32 min Scan# 358
 Delta R.T. 0.00 min
 Lab File: VU027856.D
 Acq: 29 Oct 2018 15:17

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBS9

Tgt Ion: 43 Resp: 3689
 Ion Ratio Lower Upper
 43 100
 58 28.5 0.0 57.4

