

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102918\
 Data File : VU027861.D
 Acq On : 29 Oct 2018 17:13
 Operator : MD/SY
 Sample : J5716-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBT2

Quant Time: Oct 30 04:10:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 02:27:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	111749	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	102245	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	48515	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	33030	37.99	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.98%
7) Chloroethane-d5	1.68	69	27276	40.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.50%
11) 1,1-Dichloroethene-d2	2.27	63	48371	30.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.78%
21) 2-Butanone-d5	4.18	46	65567	88.49	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.49%
24) Chloroform-d	4.65	84	65370	41.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.64%
26) 1,2-Dichloroethane-d4	5.31	65	46699	43.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.30%
32) Benzene-d6	5.34	84	129162	44.36	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.72%
36) 1,2-Dichloropropane-d6	6.33	67	46198	44.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.88%
41) Toluene-d8	7.57	98	118466	44.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.22%
43) trans-1,3-Dichloropropene-	7.85	79	21747	43.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.16%
47) 2-Hexanone-d5	8.31	63	49628	93.29	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.29%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	59826	44.57	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.14%
64) 1,2-Dichlorobenzene-d4	11.86	152	44123	44.40	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.80%


Target Compounds					Qvalue
13) Acetone	2.32	43	2789	5.40 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102918\
Data File : VU027861.D
Acq On : 29 Oct 2018 17:13
Operator : MD/SY
Sample : J5716-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBT2

Quant Time: Oct 30 04:10:00 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 02:27:31 2018
Response via : Initial Calibration

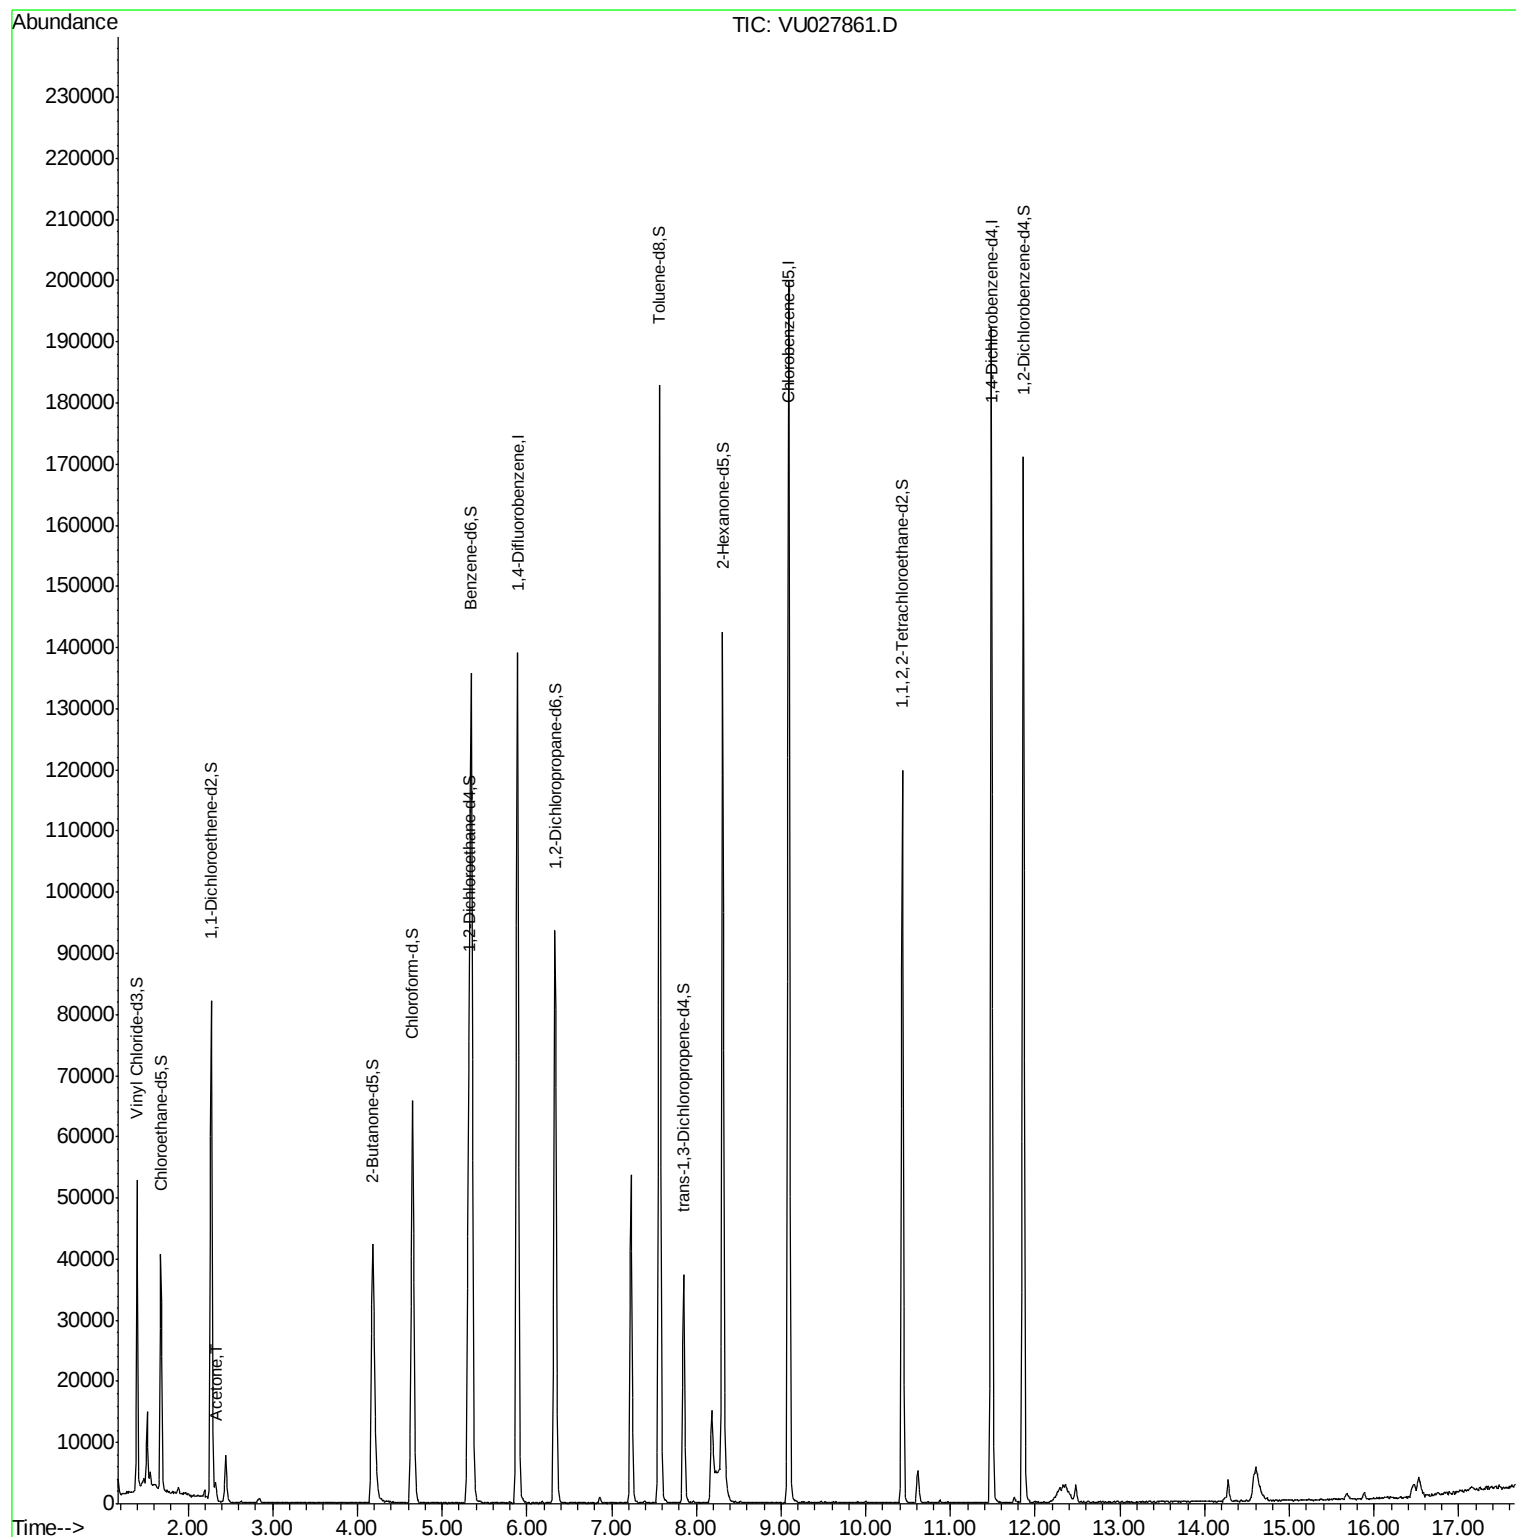

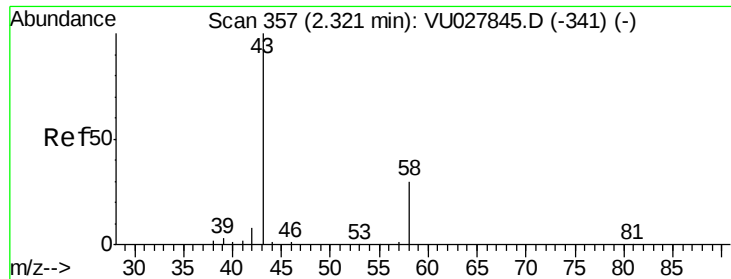

#13

Acetone

Concen: 5.40 ug/L

RT: 2.32 min Scan# 358

Delta R.T. 0.00 min

Lab File: VU027861.D

Acq: 29 Oct 2018 17:13

Instrument :
MSVOA_U
ClientSampleId :
ETBT2

Tgt Ion: 43 Resp: 2789

Ion Ratio Lower Upper

43 100

58 26.4 0.0 57.4

