

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102918\
 Data File : VU027862.D
 Acq On : 29 Oct 2018 17:36
 Operator : MD/SY
 Sample : J5716-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETBT3

Quant Time: Oct 30 04:12:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 30 02:27:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	109172	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	101565	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	46945	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	33736	39.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.44%
7) Chloroethane-d5	1.68	69	26635	40.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.46%
11) 1,1-Dichloroethene-d2	2.27	63	48337	31.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.20%
21) 2-Butanone-d5	4.18	46	64174	88.65	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.65%
24) Chloroform-d	4.65	84	64952	42.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.06%
26) 1,2-Dichloroethane-d4	5.31	65	46271	43.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.52%
32) Benzene-d6	5.34	84	127526	44.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.18%
36) 1,2-Dichloropropane-d6	6.33	67	46694	45.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.44%
41) Toluene-d8	7.57	98	117041	43.87	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.74%
43) trans-1,3-Dichloropropene-	7.85	79	21053	41.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.96%
47) 2-Hexanone-d5	8.31	63	48034	90.89	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.89%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	60204	45.15	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.30%
64) 1,2-Dichlorobenzene-d4	11.86	152	43319	45.05	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.10%


Target Compounds					Qvalue
13) Acetone	2.32	43	2485	4.93 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102918\
Data File : VU027862.D
Acq On : 29 Oct 2018 17:36
Operator : MD/SY
Sample : J5716-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETBT3

Quant Time: Oct 30 04:12:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 30 02:27:31 2018
Response via : Initial Calibration

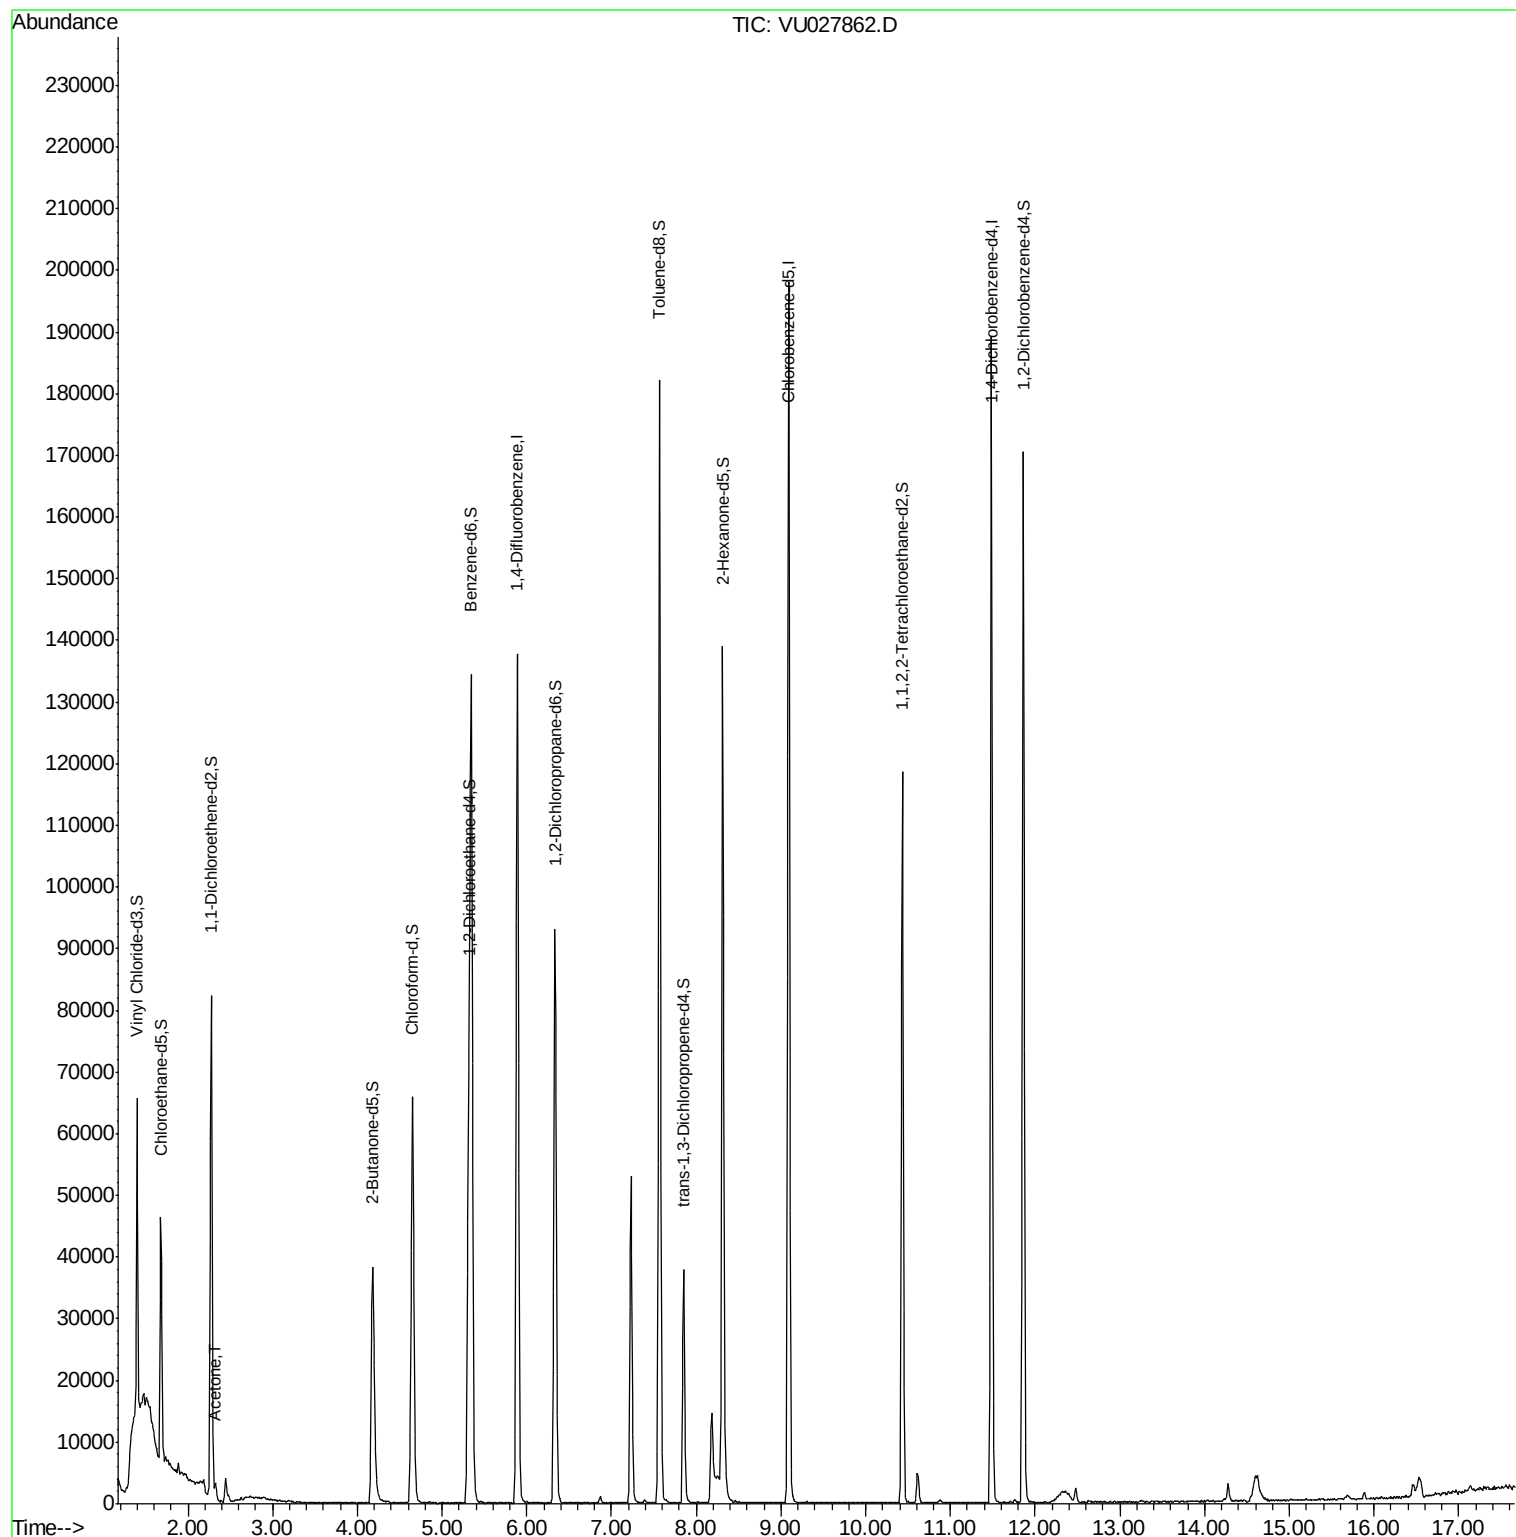

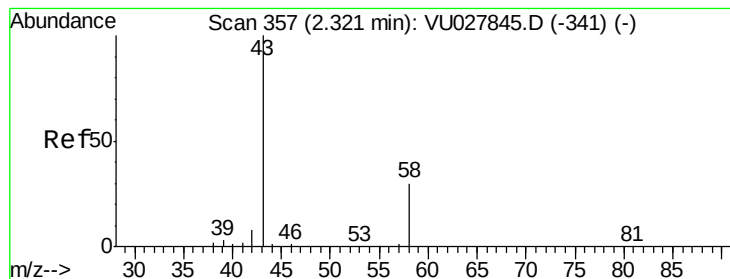

#13

Acetone

Concen: 4.93 ug/L

RT: 2.32 min Scan# 358

Delta R.T. 0.00 min

Lab File: VU027862.D

Acq: 29 Oct 2018 17:36

Instrument :
MSVOA_U
ClientSampleId :
ETBT3

Tgt Ion: 43 Resp: 2485

Ion Ratio Lower Upper

43 100

58 25.2 0.0 57.4

