


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102918\
Data File : VU027844.D
Acq On : 29 Oct 2018 07:42
Operator : MD/SY
Sample : BFB50
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Title : VOC Analysis
Last Update : Tue Oct 30 02:27:31 2018

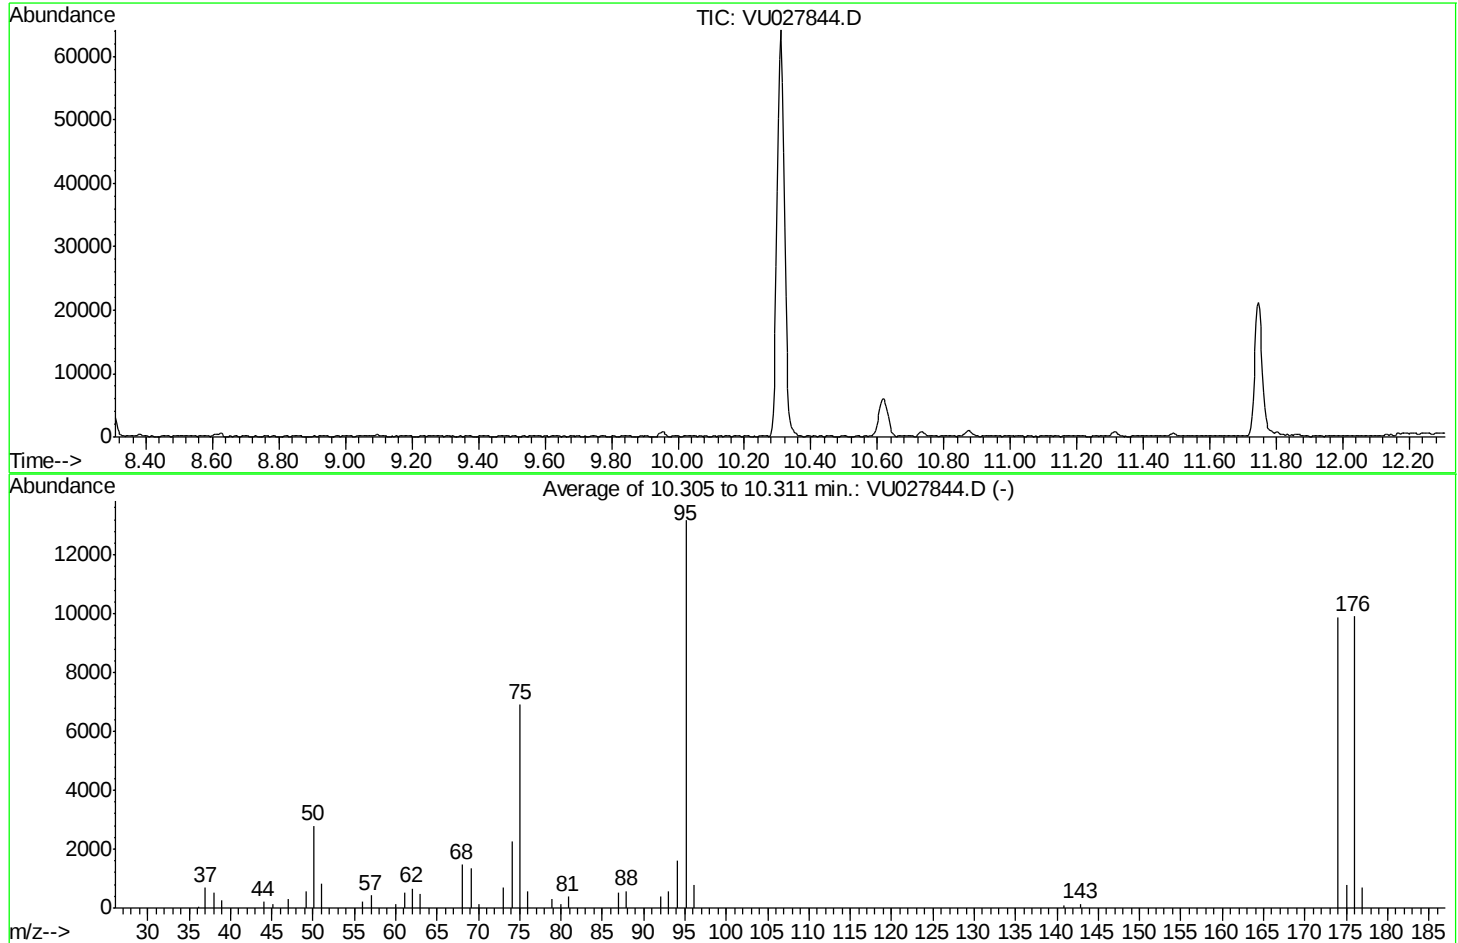

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	2806	PASS
75	95	30	80	52.5	6911	PASS
95	95	100	100	100.0	13174	PASS
96	95	5	9	5.9	781	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.0	9879	PASS
175	174	5	9	7.8	768	PASS
176	174	95	101	100.4	9914	PASS
177	176	5	9	6.8	678	PASS

m/z	Abundance
37.00	682.0
38.00	558.0
39.00	254.0
44.00	207.0
45.10	151.0
46.90	315.0
49.10	611.0
50.10	2907.0
51.10	864.0
56.00	244.0
57.00	441.0
59.90	149.0
61.10	531.0
62.00	694.0
63.00	506.0
68.00	1523.0
69.10	1423.0
70.10	125.0
73.00	757.0
74.10	2350.0
75.10	7125.0
76.00	573.0
79.00	299.0
79.90	137.0
80.90	412.0
86.90	537.0
87.90	618.0
92.00	406.0
93.00	562.0
94.00	1662.0
95.10	13626.0
96.10	788.0
140.90	123.0
142.90	134.0
174.00	10215.0
175.00	797.0
176.00	10182.0
177.00	698.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.10	123.0
37.00	634.0
38.00	532.0
39.00	235.0
44.00	228.0
45.10	129.0
46.90	298.0
49.10	520.0
50.10	2763.0
51.10	840.0
56.00	215.0
57.10	397.0
60.00	130.0
61.00	512.0
62.00	656.0
63.00	468.0
68.00	1504.0
69.10	1330.0
70.10	109.0
73.00	649.0
74.10	2183.0
75.10	6584.0
76.00	577.0
78.90	324.0
80.00	108.0
80.90	355.0
86.90	533.0
87.90	497.0
92.00	362.0
93.00	479.0
94.10	1502.0
95.10	12708.0
96.10	776.0
140.90	137.0
142.90	157.0
174.00	9349.0
175.00	722.0
176.00	9364.0
177.00	660.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z

Abundance

Instrument :

MSVOA_U

ClientSampleId :

BFB50

m/z	Abundance
37.00	731.0
38.00	526.0
39.00	250.0
44.00	200.0
45.10	152.0
47.00	267.0
49.10	609.0
50.10	2749.0
51.00	743.0
56.00	218.0
57.00	447.0
60.00	146.0
61.10	540.0
62.00	613.0
63.00	498.0
68.00	1393.0
69.10	1349.0
70.00	139.0
73.00	723.0
74.00	2286.0
75.10	7025.0
76.00	560.0
78.90	272.0
79.90	147.0
80.80	397.0
87.00	548.0
87.90	593.0
92.00	416.0
93.00	641.0
94.00	1661.0
95.10	13188.0
96.00	780.0
142.90	118.0
174.00	10074.0
175.00	785.0
176.00	10196.0
177.00	678.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50