



1,2,4-Trichlorobenzene

Response Ratio

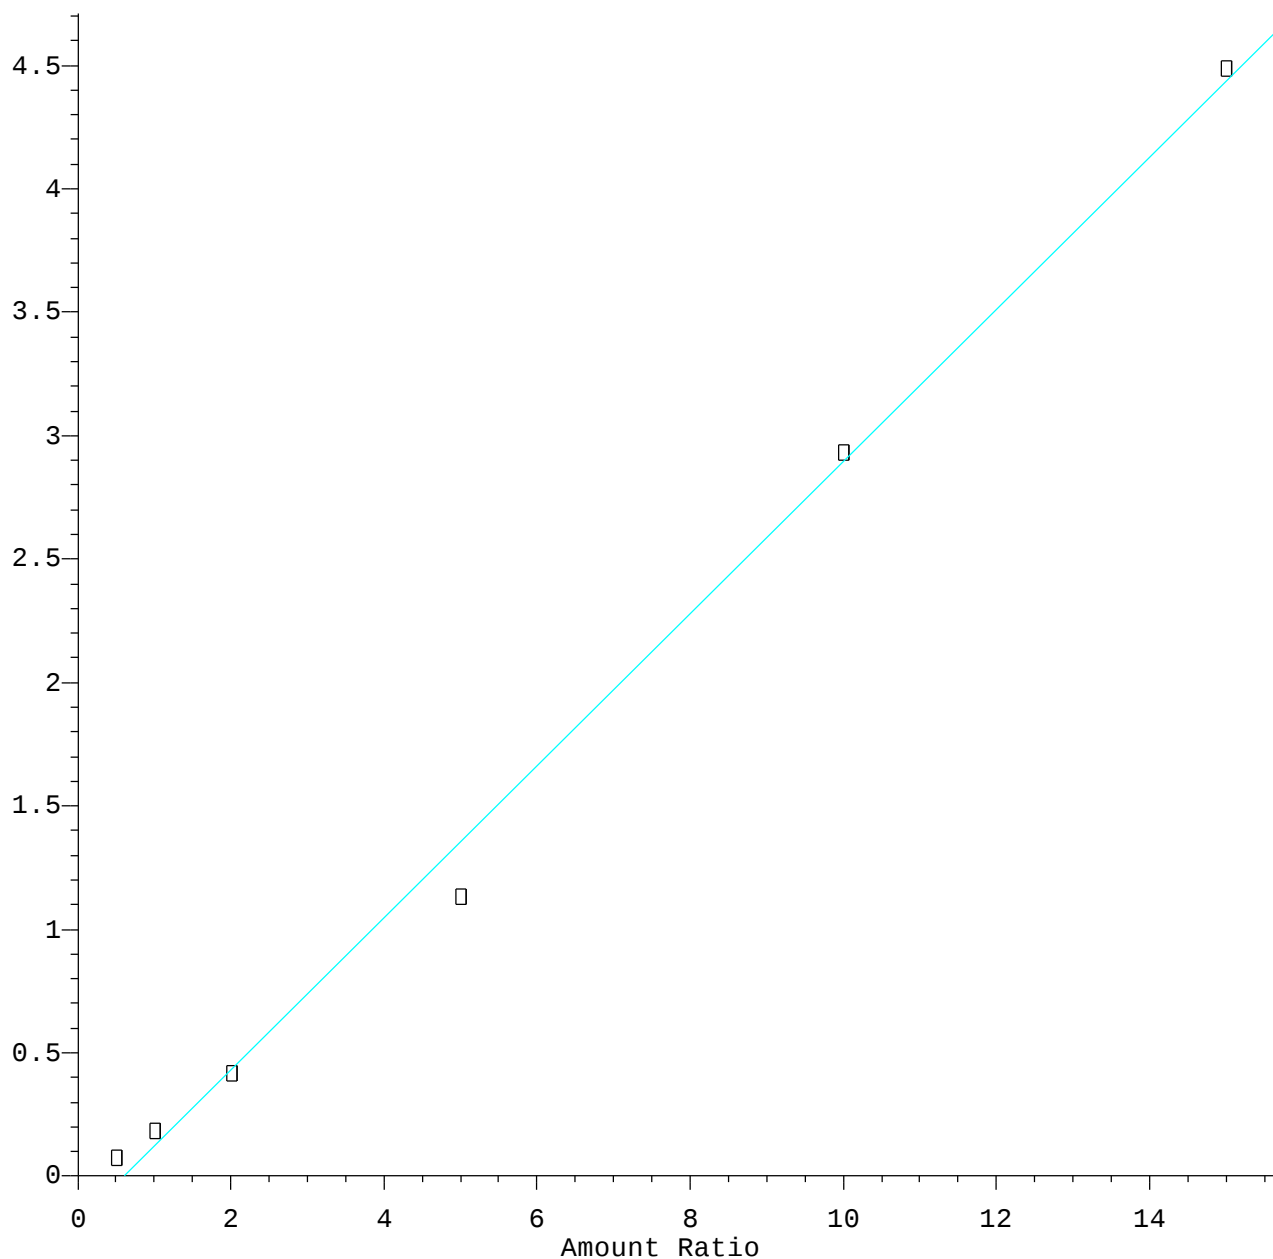

Resp Ratio = $3.08 \times 10^{-1} \times \text{Amt} - 1.84 \times 10^{-1}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Calibration Table Last Updated: Wed Oct 30 07:13:39 2019

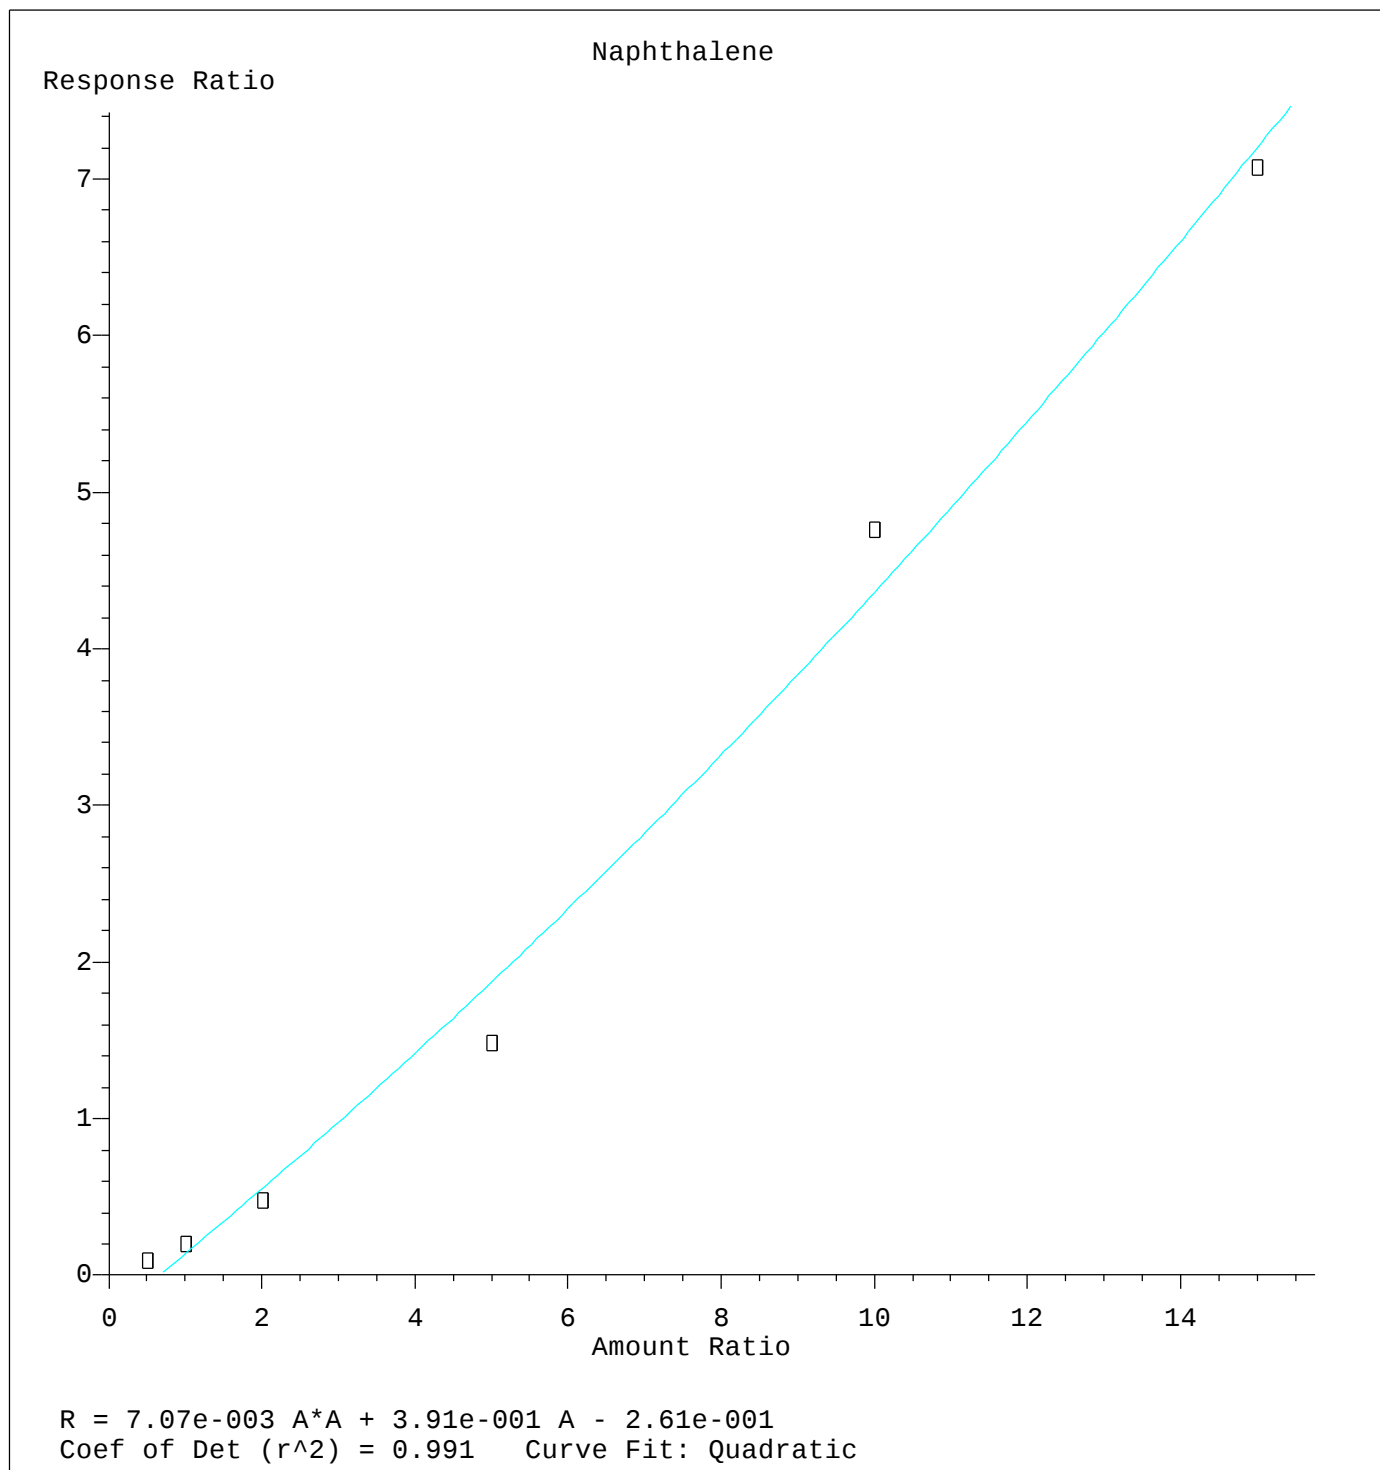

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Calibration Table Last Updated: Wed Oct 30 07:13:39 2019

1,2,3-Trichlorobenzene

Response Ratio

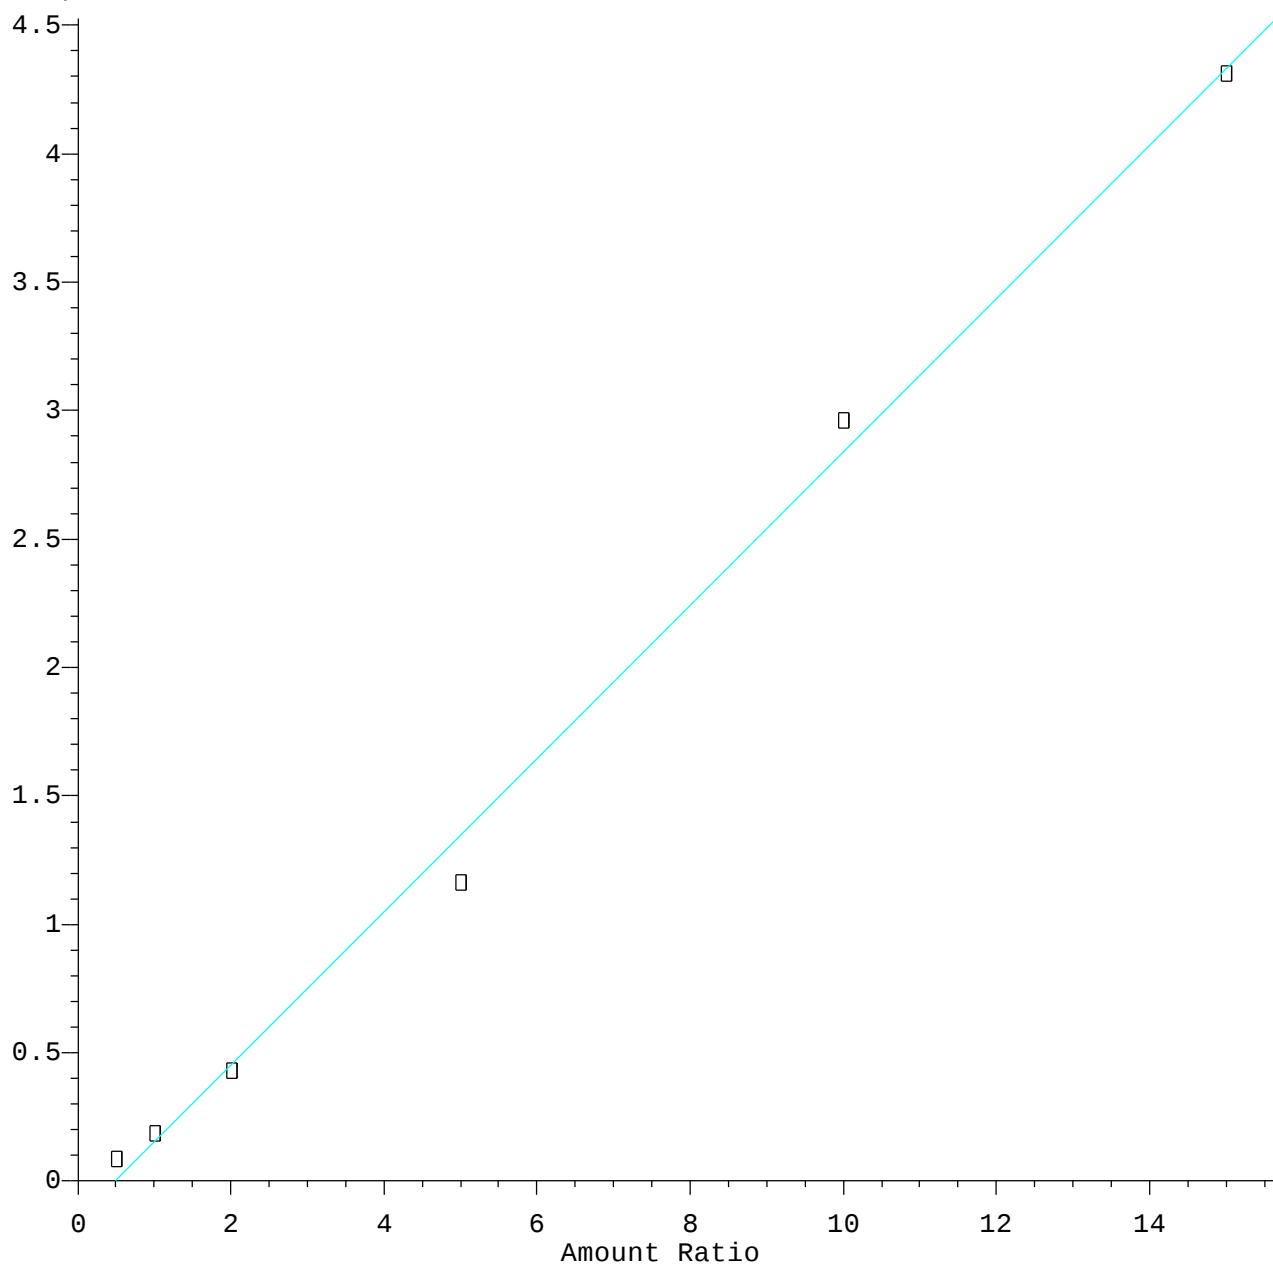


Resp Ratio = $2.98 \times 10^{-1} \times \text{Amt} - 1.44 \times 10^{-1}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Calibration Table Last Updated: Wed Oct 30 07:13:39 2019

Iodomethane

Response Ratio

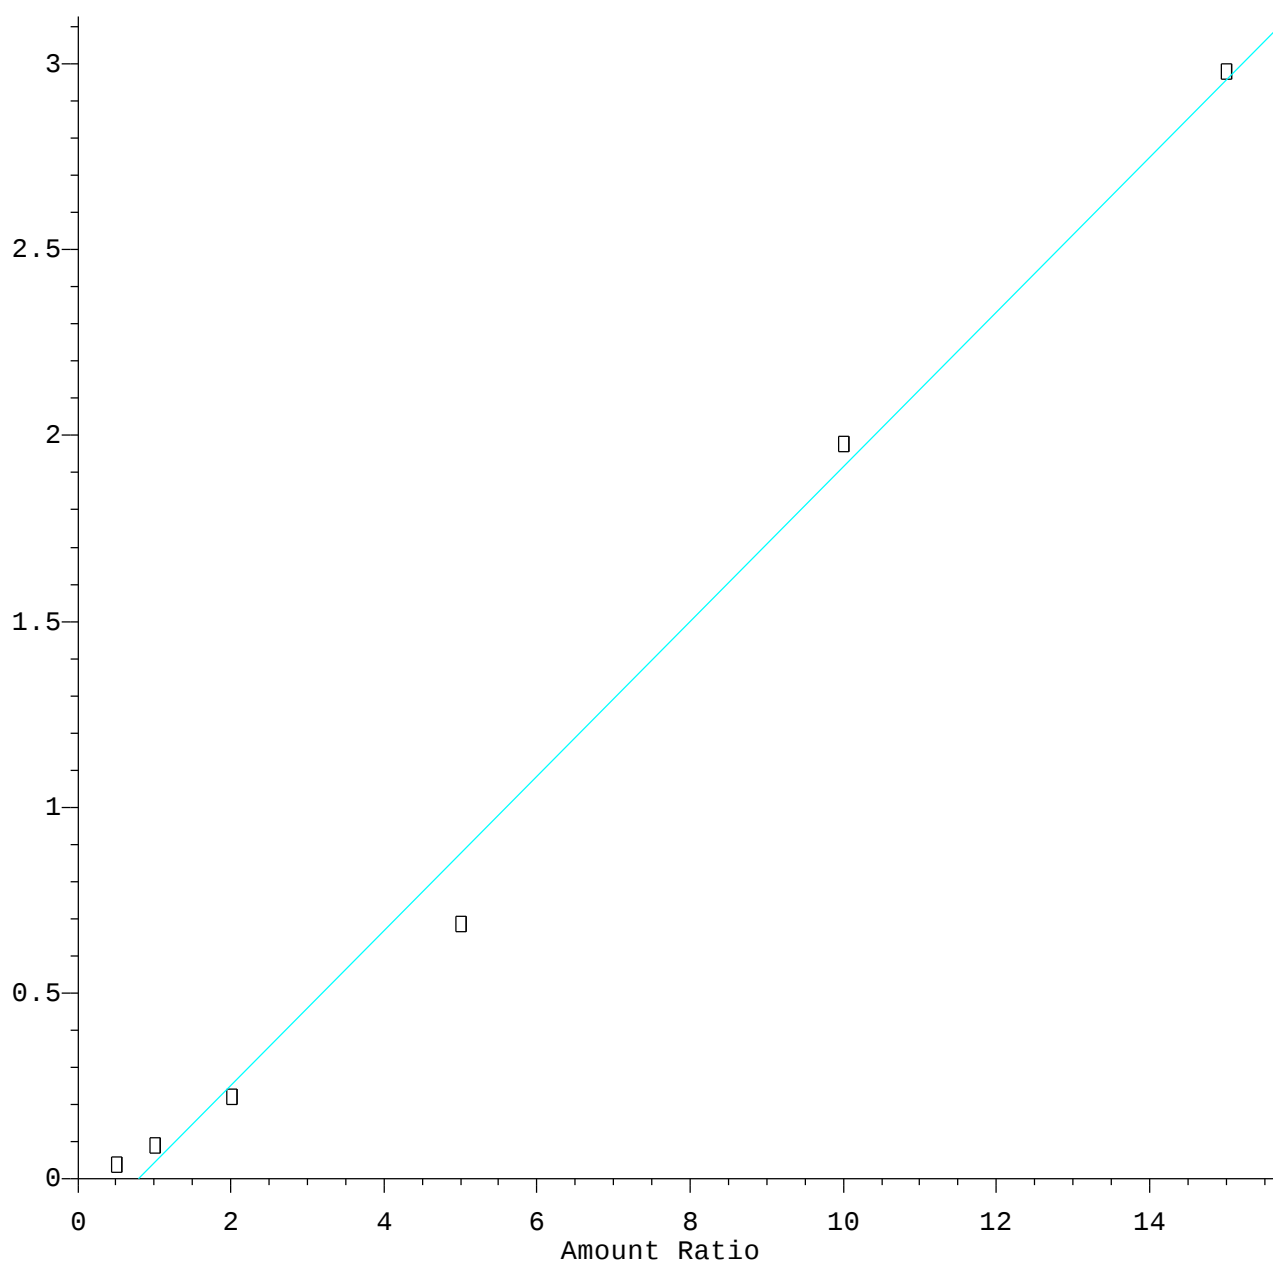

Resp Ratio = $2.08 \times 10^{-1} \times \text{Amt} - 1.64 \times 10^{-1}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Calibration Table Last Updated: Wed Oct 30 07:13:39 2019