

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102919\
 Data File : VU035542.D
 Acq On : 29 Oct 2019 16:38
 Operator : JC/SP
 Sample : VU1029WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1029WBL01

Quant Time: Oct 30 06:12:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Oct 30 05:38:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	6.16	96	68429	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.67	95	21451	0.87	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.00%	
68) 1,2-Dichlorobenzene-d4	12.22	152	21200	0.81	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.00%	


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102919\
Data File : VU035542.D
Acq On : 29 Oct 2019 16:38
Operator : JC/SP
Sample : VU1029WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1029WBL01

Quant Time: Oct 30 06:12:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Oct 30 05:38:55 2019
Response via : Initial Calibration

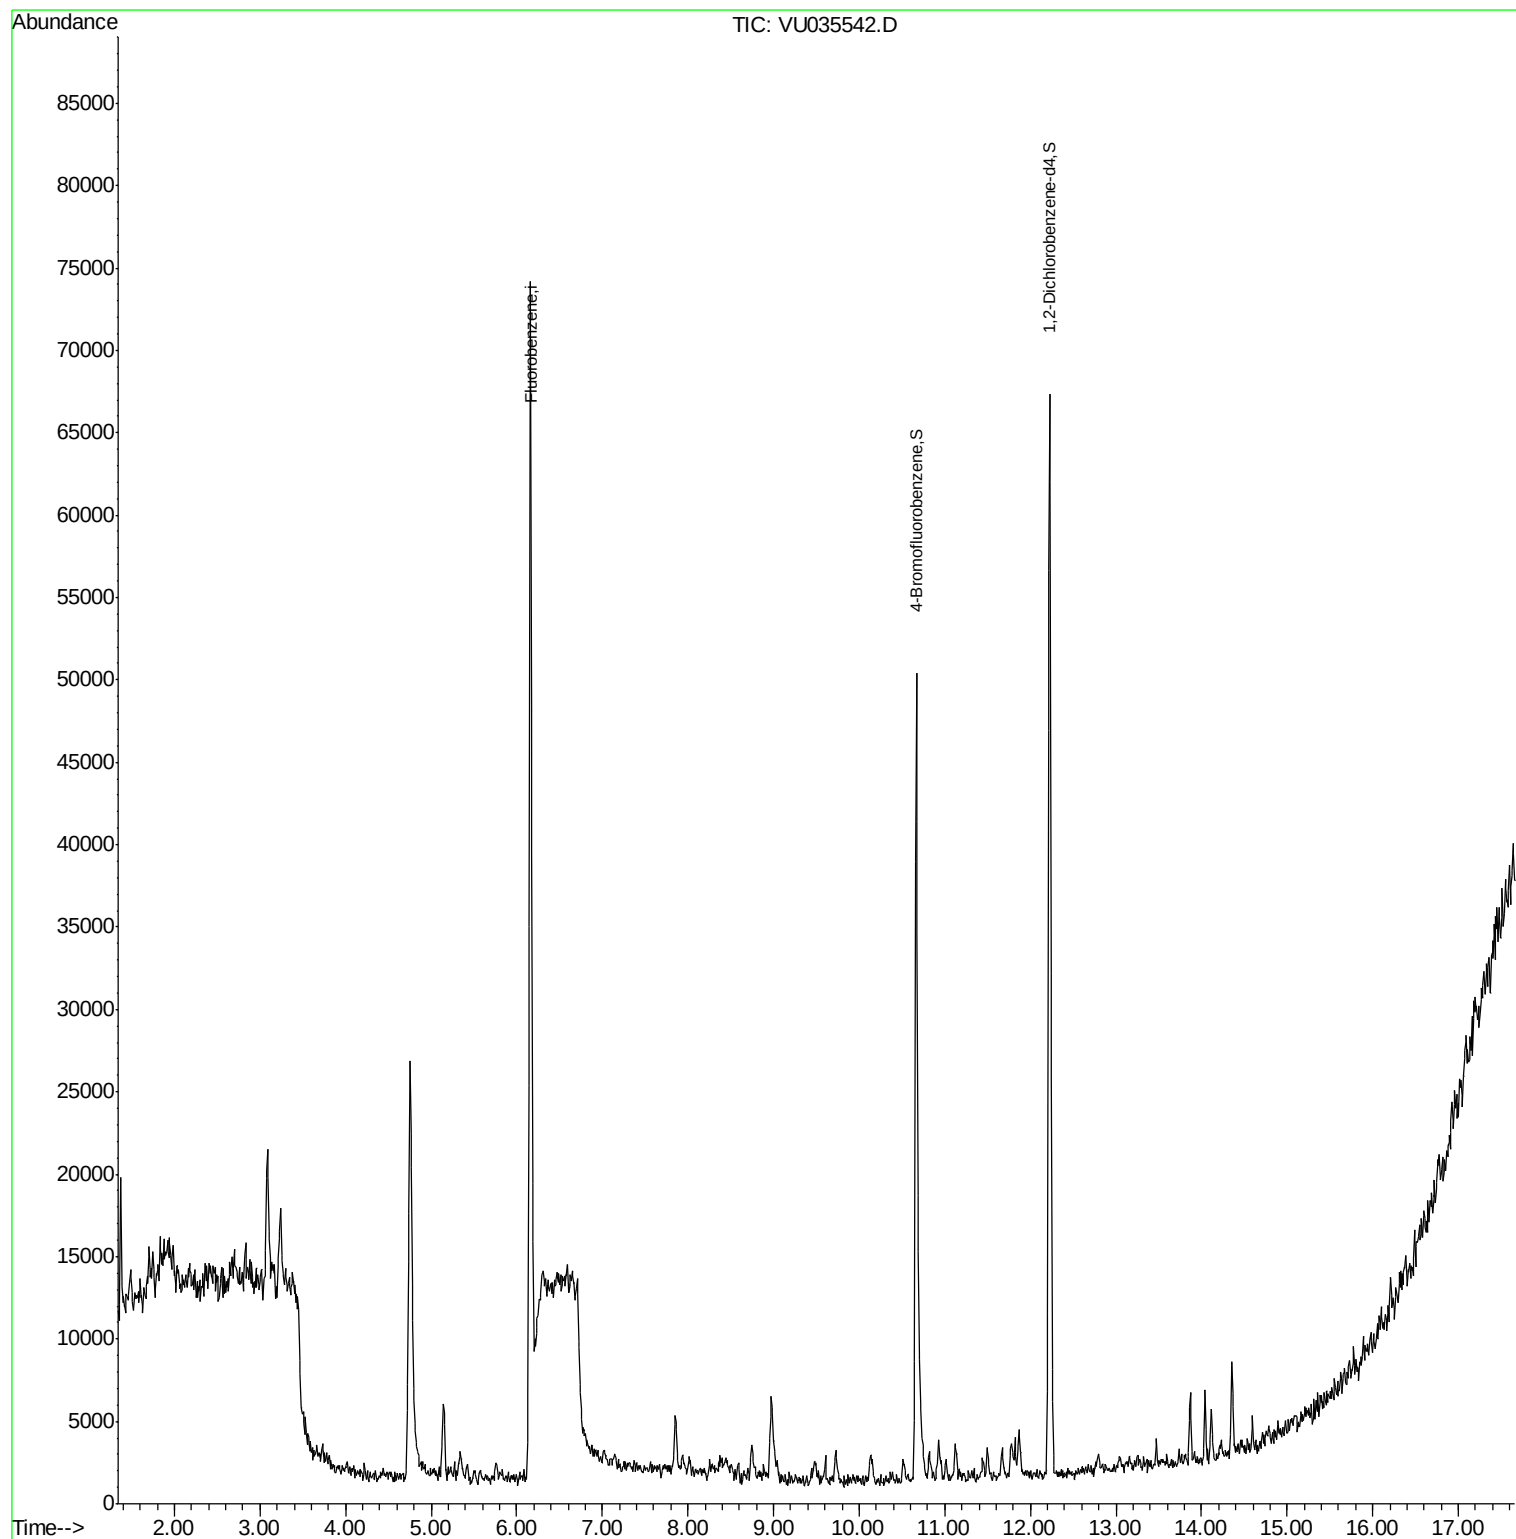

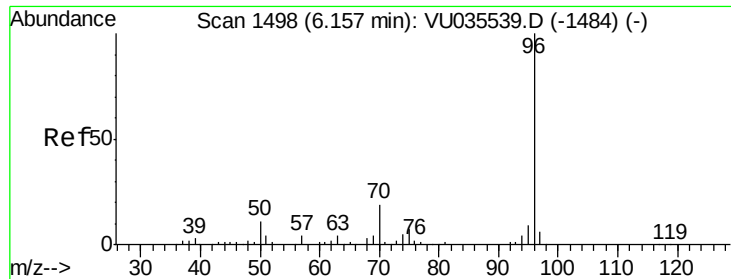

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.16 min Scan# 1499

Delta R.T. 0.00 min

Lab File: VU035542.D

Acq: 29 Oct 2019 16:38

Instrument :

MSVOA_U

ClientSampleId :

VU1029WBL01

Tgt Ion: 96 Resp: 68429


Ion Ratio Lower Upper

96 100

70 19.9 15.8 23.8

95 9.4 7.4 11.2

97 6.3 0.0 0.0#



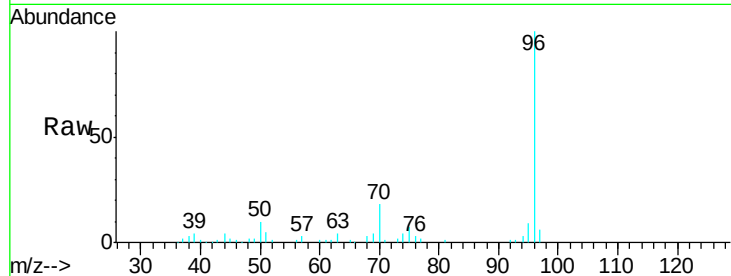


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

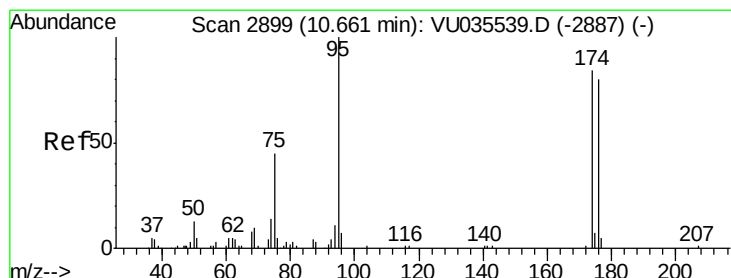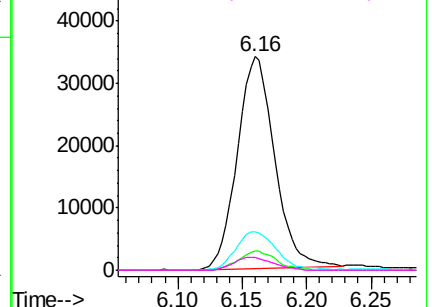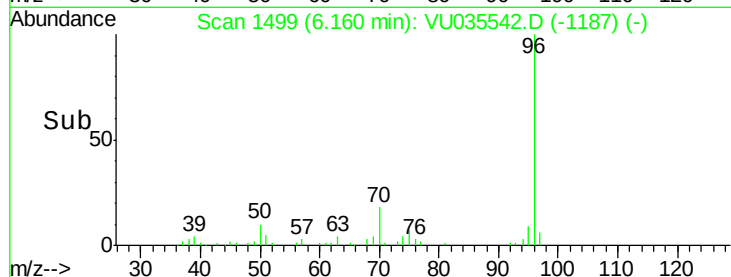

#57

4-Bromofluorobenzene

Concen: 0.871 ug/l

RT: 10.67 min Scan# 2901

Delta R.T. 0.01 min

Lab File: VU035542.D

Acq: 29 Oct 2019 16:38


Tgt Ion: 95 Resp: 21451

Ion Ratio Lower Upper

95 100

174 93.9 70.2 105.4



176 86.4 67.7 101.5

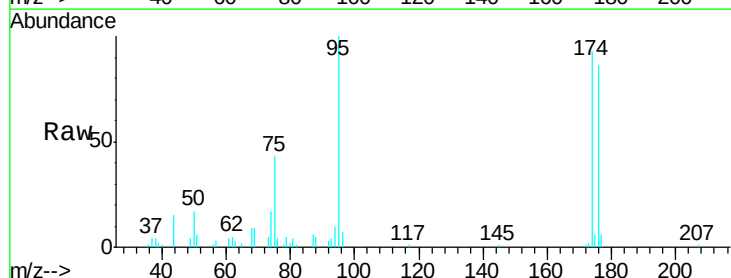


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

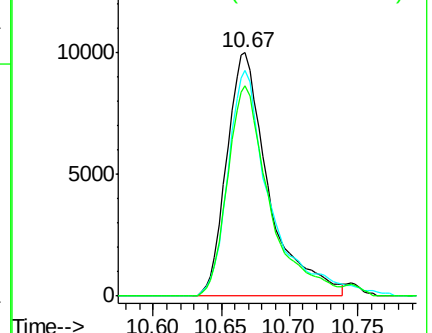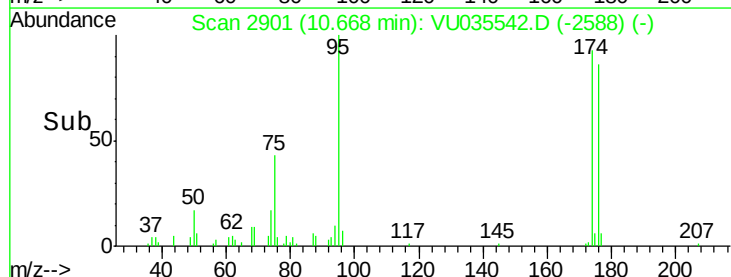

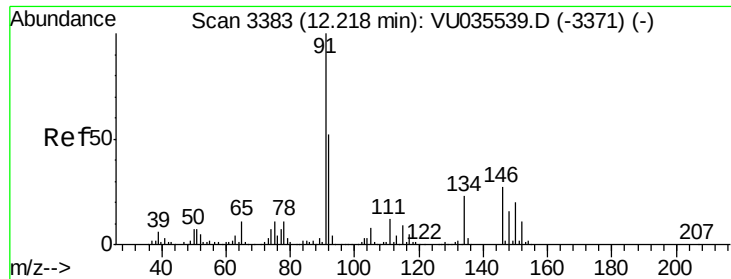

#68

1,2-Dichlorobenzene-d4

Concen: 0.810 ug/l

RT: 12.22 min Scan# 3385

Delta R.T. 0.01 min

Lab File: VU035542.D


Acq: 29 Oct 2019 16:38

Instrument :

MSVOA_U

ClientSampleId :

VU1029WBL01

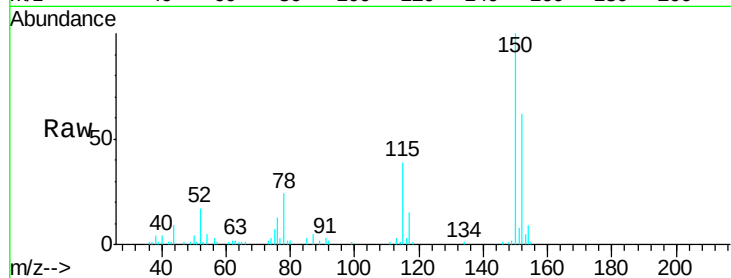

Tgt Ion:152 Resp: 21200

Ion Ratio Lower Upper

152 100

115 61.5 0.0 250.6

150 163.3 0.0 656.8

