

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102919\
 Data File : VU035542.D
 Acq On : 29 Oct 2019 16:38
 Operator : JC/SP
 Sample : VU1029WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1029WBL01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.755	1045	1062	1081	rBV2	25346	75495	48.05%	13.907%
2	5.137	1171	1181	1182	rBV6	4286	4629	2.95%	0.853%
3	6.160	1484	1499	1514	rBV2	72709	157112	100.00%	28.942%
4	7.854	2017	2026	2036	rVB5	3055	5295	3.37%	0.975%
5	8.739	2294	2301	2303	rBV3	2141	2283	1.45%	0.421%
6	8.976	2363	2375	2383	rBV5	5000	11286	7.18%	2.079%
7	9.729	2599	2609	2615	rBV5	1922	3205	2.04%	0.590%
8	10.513	2847	2853	2856	rBV2	1445	1763	1.12%	0.325%
9	10.668	2890	2901	2923	rBV2	48912	103338	65.77%	19.036%
10	10.819	2940	2948	2951	rBV5	1657	1989	1.27%	0.366%
11	10.928	2976	2982	2985	rBV5	1960	1895	1.21%	0.349%
12	11.015	3001	3009	3016	rBV6	1246	1913	1.22%	0.352%
13	11.671	3205	3213	3220	rBV5	1660	2389	1.52%	0.440%
14	11.774	3239	3245	3246	rBV3	1940	1895	1.21%	0.349%
15	11.864	3267	3273	3280	rBV8	2207	3316	2.11%	0.611%
16	12.224	3371	3385	3402	rBV2	65559	134807	85.80%	24.833%
17	13.870	3887	3897	3905	rBV5	4399	6804	4.33%	1.253%
18	14.044	3940	3951	3957	rBV5	4616	6883	4.38%	1.268%
19	14.115	3967	3973	3985	rVB4	3138	4924	3.13%	0.907%
20	14.356	4039	4048	4055	rBV5	5928	9352	5.95%	1.723%
21	14.597	4116	4123	4130	rBV5	2195	2278	1.45%	0.420%


Sum of corrected areas: 542851

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102919\
Data File : VU035542.D
Acq On : 29 Oct 2019 16:38
Operator : JC/SP
Sample : VU1029WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1029WBL01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

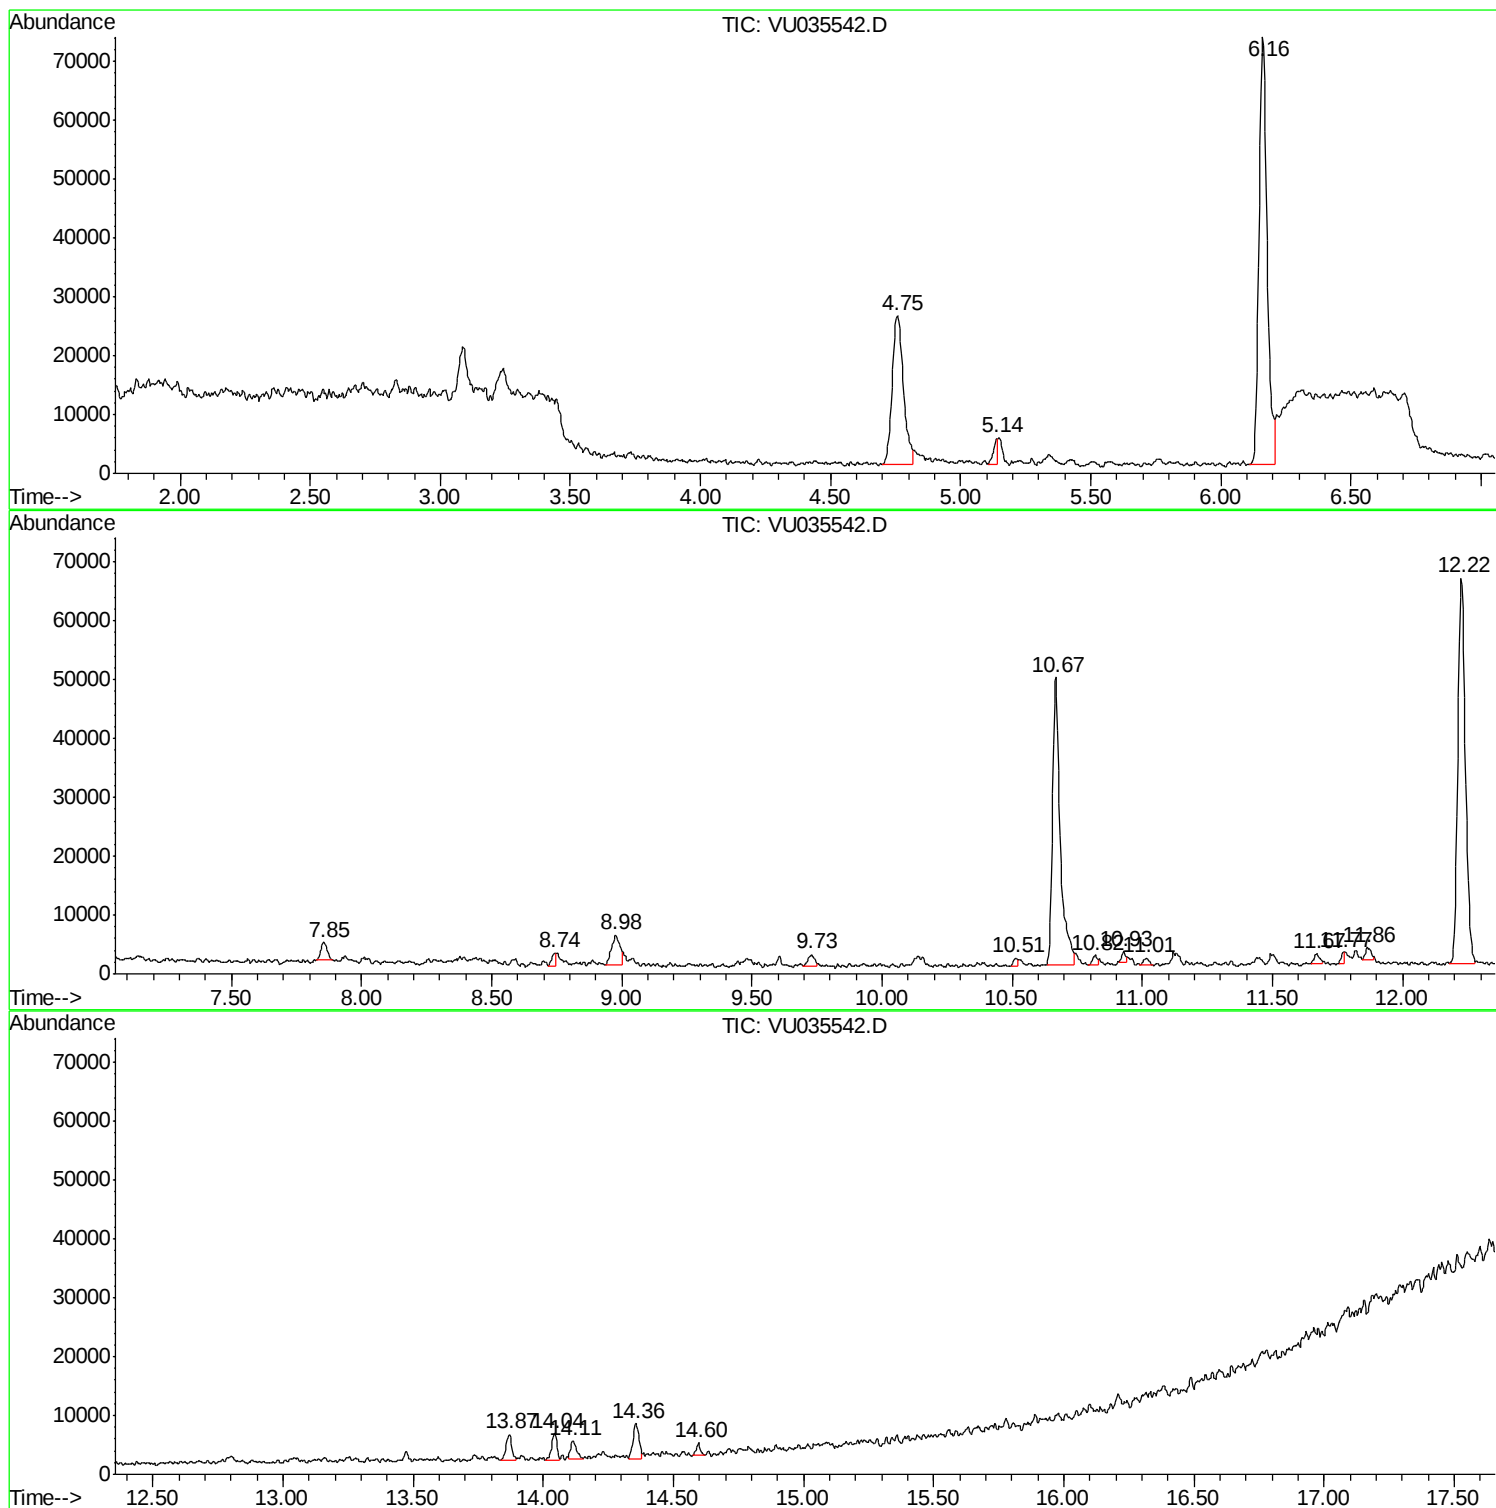

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102919\
Data File : VU035542.D
Acq On : 29 Oct 2019 16:38
Operator : JC/SP
Sample : VU1029WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1029WBL01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : \\74.0.250.170\TERASTORAGE\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102919\
Data File : VU035542.D
Acq On : 29 Oct 2019 16:38
Operator : JC/SP
Sample : VU1029WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1029WBL01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc