


Data Path : \\74.0.250.170\terastorage\voasrv\HPCHEM1\MSVOA_U\Data\VU102919\
Data File : VU035534.D
Acq On : 29 Oct 2019 09:10
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Oct 30 07:13:39 2019

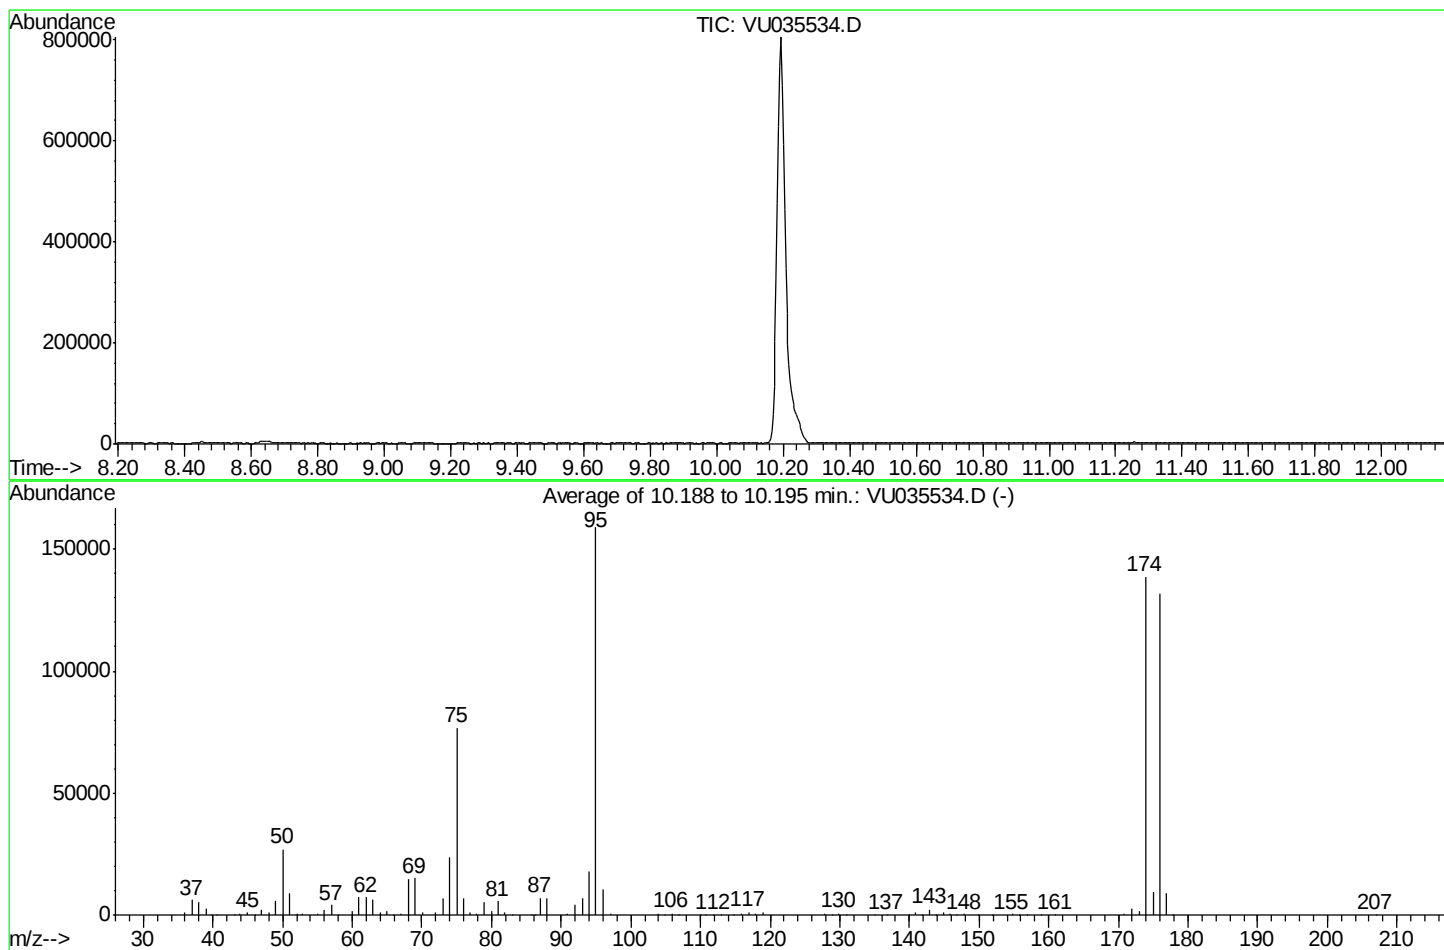

AutoFind: Scans 2752, 2753, 2754; Background Corrected with Scan 2739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	27050	PASS
75	95	30	60	48.4	76888	PASS
95	95	100	100	100.0	158976	PASS
96	95	5	9	6.5	10319	PASS
173	174	0.00	2	1.3	1832	PASS
174	95	50	100	87.2	138592	PASS
175	174	5	9	7.0	9666	PASS
176	174	95	101	95.1	131768	PASS
177	176	5	9	6.6	8750	PASS