

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102921\
 Data File : VU045459.D
 Acq On : 29 Oct 2021 13:26
 Operator : SY/MD
 Sample : M4360-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BP-VPB-RW9-GW-218-220

Quant Time: Oct 30 04:04:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U102821W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 29 11:09:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.378	168	194915	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	378889	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	364747	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.815	152	175516	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.706	65	163172	51.421	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.840%			
35) Dibromofluoromethane	5.295	113	119843	49.745	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.480%			
50) Toluene-d8	7.902	98	484187	51.252	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 102.500%			
62) 4-Bromofluorobenzene	10.635	95	180840	50.234	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 100.460%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.385	85	77	0.403	ug/l #	43
3) Chloromethane	1.520	50	900	0.232	ug/l #	81
10) Methyl Iodide	2.735	142	248	9.451	ug/l #	43
15) Acrylonitrile	3.333	53	682	0.411	ug/l #	86
16) Acetone	2.642	43	3850	2.672	ug/l	98
17) Carbon Disulfide	2.800	76	2377	0.367	ug/l	99
25) 2-Butanone	4.726	43	1494	0.687	ug/l	97
29) Tetrahydrofuran	5.063	42	383	0.272	ug/l #	30
31) Cyclohexane	5.382	56	4774	1.010	ug/l #	1
36) 1,1-Dichloropropene	5.378	75	17179	4.763	ug/l #	50
38) Carbon Tetrachloride	5.378	117	20487	6.513	ug/l #	16
49) 1,4-Dioxane	6.999	88	172	2.169	ug/l #	97
51) 4-Methyl-2-Pentanone	7.796	43	1303	0.306	ug/l	93
56) Ethyl methacrylate	8.340	69	149	1.670	ug/l #	84
59) 2-Hexanone	8.690	43	1487	0.451	ug/l	94
68) m/p-Xylenes	9.696	106	1280	0.268	ug/l	95
70) Styrene	10.118	104	1107	1.102	ug/l	93
71) Bromoform	10.295	173	96	2.029	ug/l #	29
74) N-amyl acetate	10.320	43	347	1.210	ug/l #	63
76) 1,2,3-Trichloropropane	10.635	75	93177	19.925	ug/l #	42
81) trans-1,4-Dichloro-2-b...	10.635	75	93177	55.353	ug/l #	12
82) 4-Chlorotoluene	11.098	91	2304	0.235	ug/l	89
86) p-Isopropyltoluene	11.796	119	1789	0.347	ug/l #	71
87) 1,3-Dichlorobenzene	11.748	146	1664	0.305	ug/l	92
88) 1,4-Dichlorobenzene	11.748	146	1664	0.299	ug/l	94
89) n-Butylbenzene	12.214	91	3038	1.211	ug/l	97
91) 1,2-Dichlorobenzene	12.214	146	1249	0.229	ug/l	94
93) 1,2,4-Trichlorobenzene	13.844	180	2081	0.570	ug/l	95
94) Hexachlorobutadiene	14.024	225	526	0.396	ug/l	89
95) Naphthalene	14.092	128	6118	0.523	ug/l	96
96) 1,2,3-Trichlorobenzene	14.333	180	2031	0.552	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102921\
Data File : VU045459.D
Acq On : 29 Oct 2021 13:26
Operator : SY/MD
Sample : M4360-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220

Quant Time: Oct 30 04:04:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U102821W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 29 11:09:42 2021
Response via : Initial Calibration

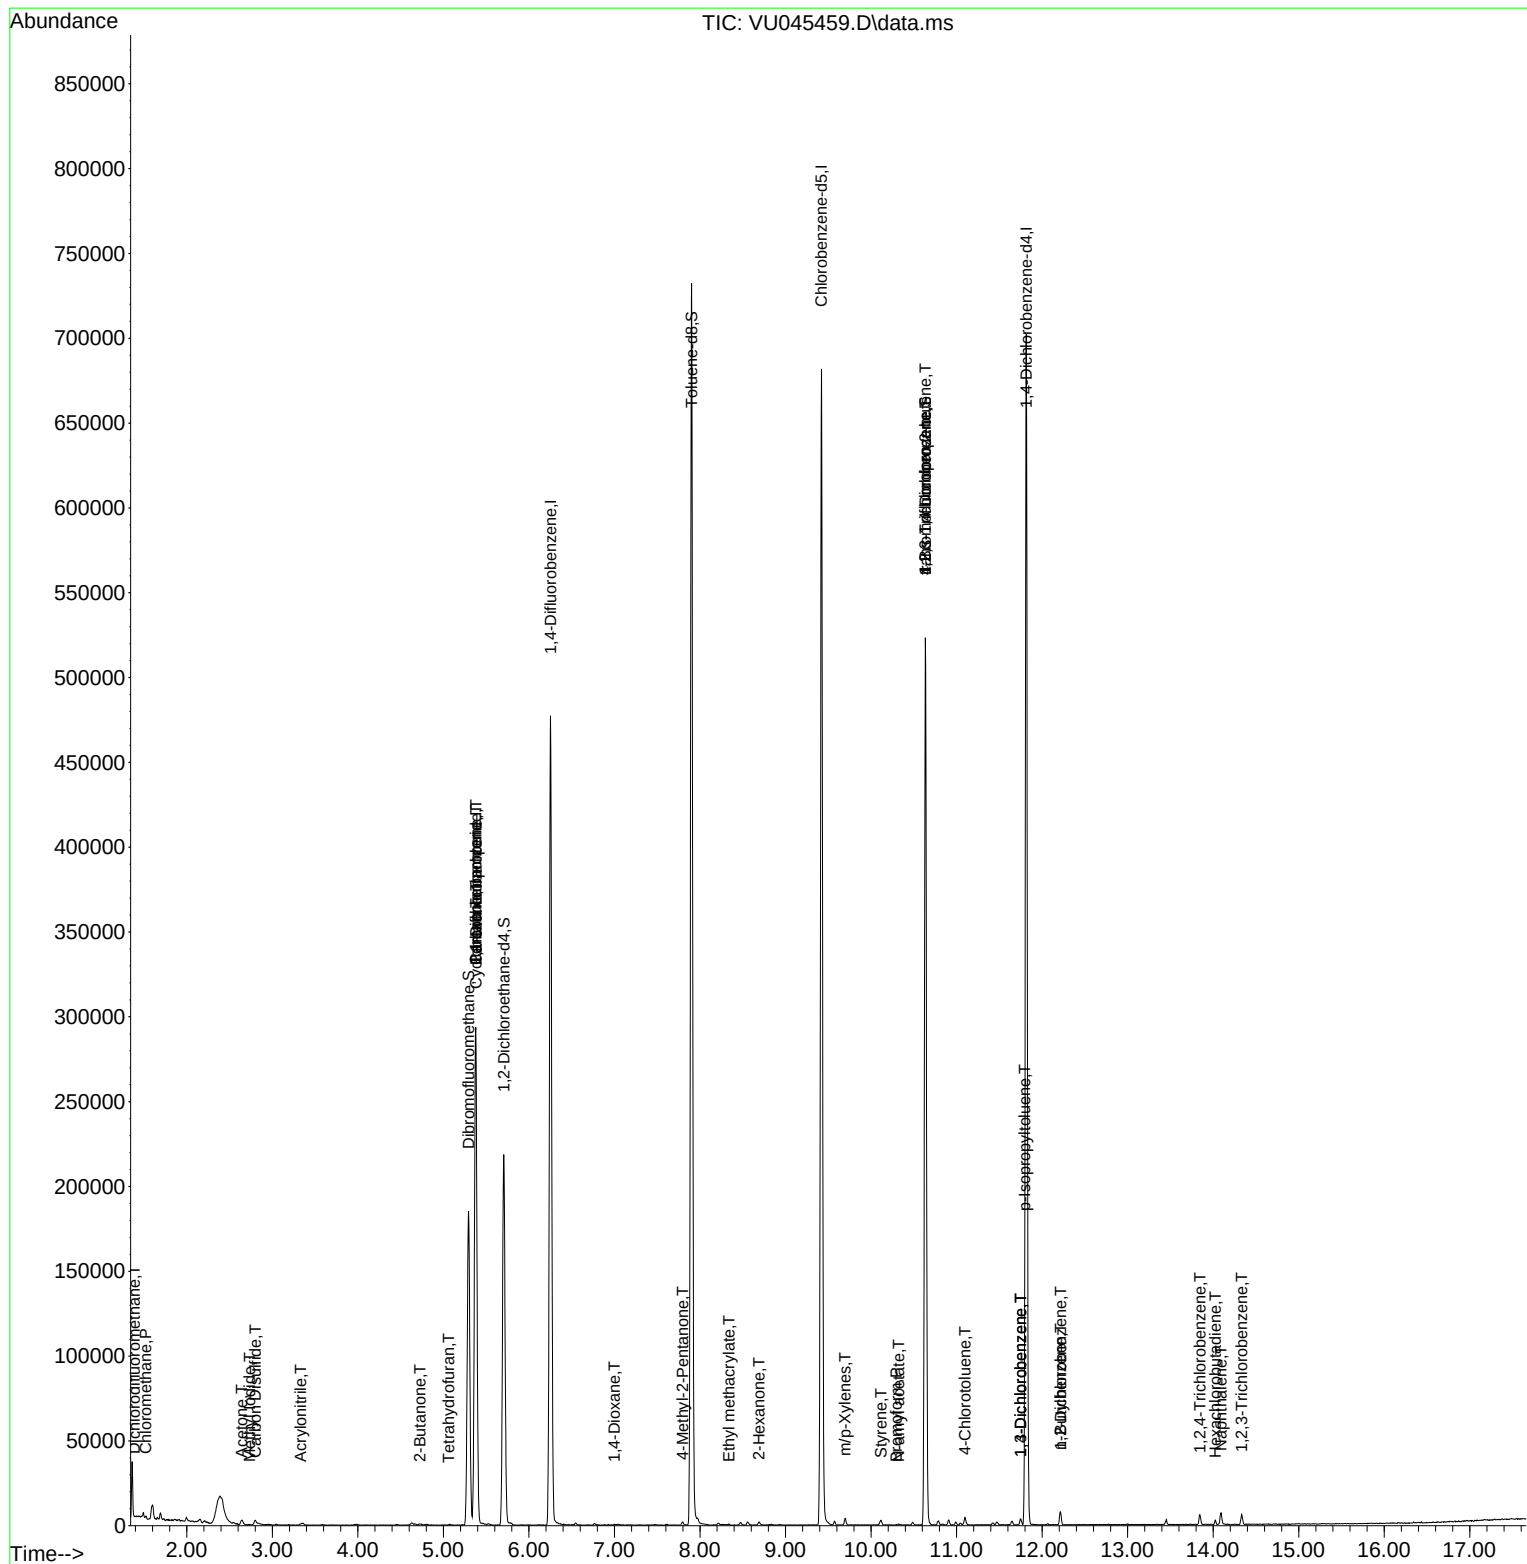



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.378 min Scan# 11

Delta R.T. -0.001 min

Lab File: VU045459.D

Acq: 29 Oct 2021 13:26

Instrument :

MSVOA_U

ClientSampleId :





BP-VPB-RW9-GW-218-220

Tgt Ion:168 Resp: 194915

Ion Ratio Lower Upper

168 100

99 63.0 51.0 76.6

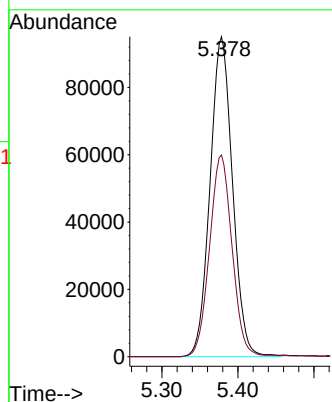

#2

Dichlorodifluoromethane

Concen: 0.403 ug/l

RT: 1.385 min Scan# 14

Delta R.T. -0.000 min

Lab File: VU045459.D




Acq: 29 Oct 2021 13:26


Tgt Ion: 85 Resp: 77

Ion Ratio Lower Upper

85 100

87 0.0 15.9 47.7#


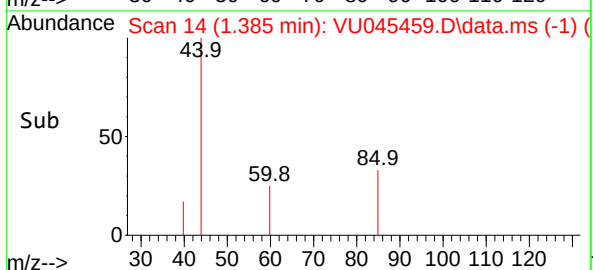




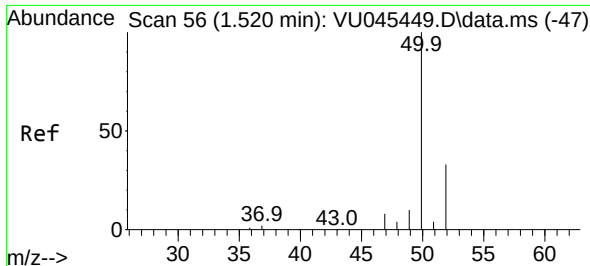

#3
Chloromethane
Concen: 0.232 ug/l
RT: 1.520 min Scan# 50
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion: 50 Resp: 900
Ion Ratio Lower Upper
50 100
52 44.2 26.6 40.0#

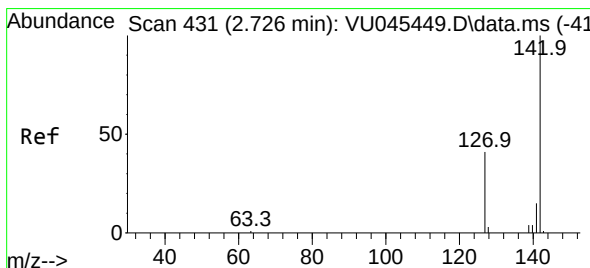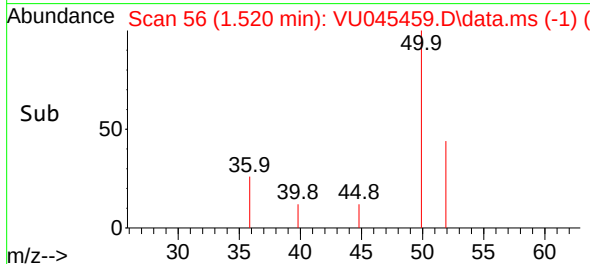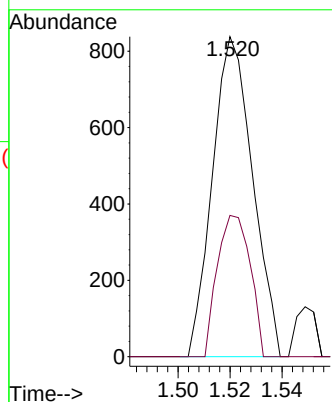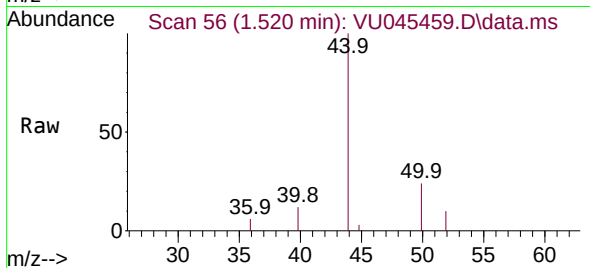

#10
Methyl Iodide
Concen: 9.451 ug/l
RT: 2.735 min Scan# 434
Delta R.T. 0.009 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 142 Resp: 248
Ion Ratio Lower Upper
142 100
127 0.0 32.2 48.2#
141 0.0 11.3 16.9#


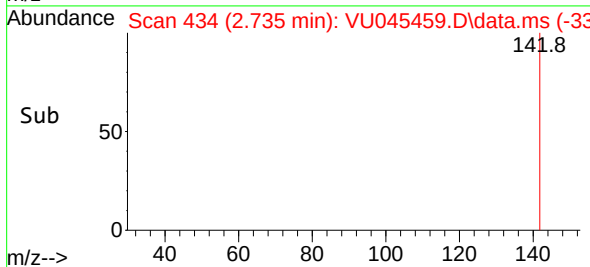

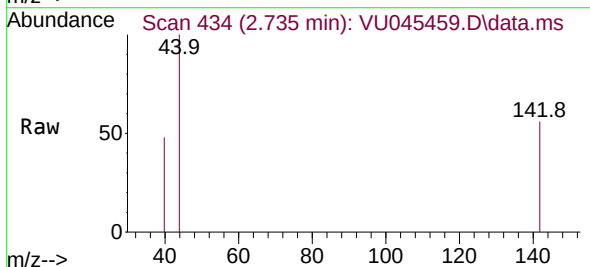




#15
Acrylonitrile
Concen: 0.411 ug/l
RT: 3.333 min Scan# 616
Delta R.T. 0.013 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion: 53 Resp: 682
Ion Ratio Lower Upper
53 100
52 81.8 66.6 100.0
51 10.0 28.4 42.6#

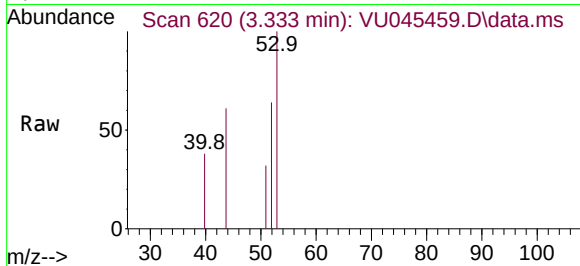

#16
Acetone
Concen: 2.672 ug/l
RT: 2.642 min Scan# 405
Delta R.T. 0.003 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 43 Resp: 3850
Ion Ratio Lower Upper
43 100
58 31.5 26.2 39.2


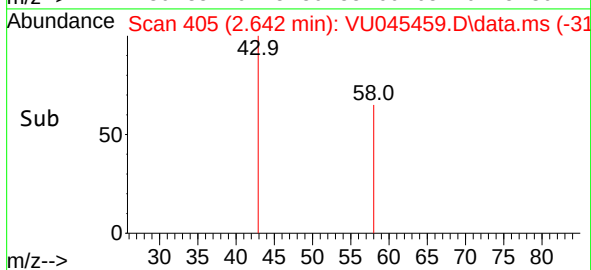

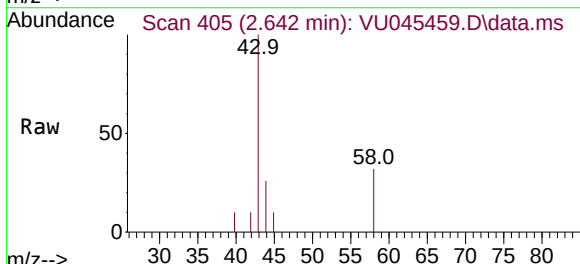




#17
Carbon Disulfide
Concen: 0.367 ug/l
RT: 2.800 min Scan# 41
Delta R.T. 0.003 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion: 76 Resp: 2377
Ion Ratio Lower Upper
76 100
78 9.5 7.3 10.9

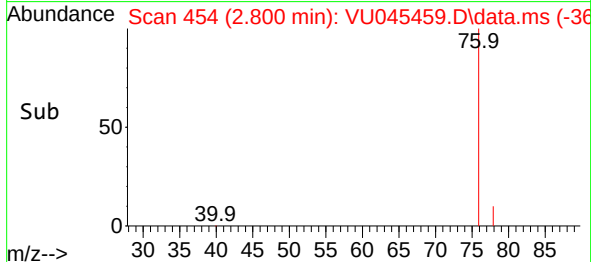

#25
2-Butanone
Concen: 0.687 ug/l
RT: 4.726 min Scan# 1053
Delta R.T. 0.016 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 43 Resp: 1494
Ion Ratio Lower Upper
43 100
72 26.0 22.0 33.0

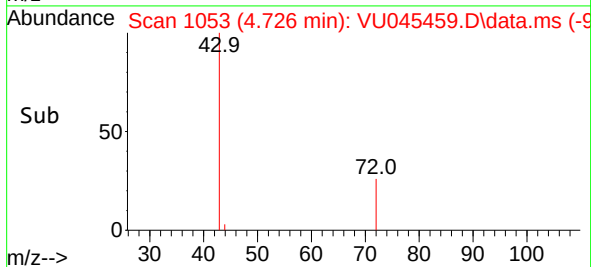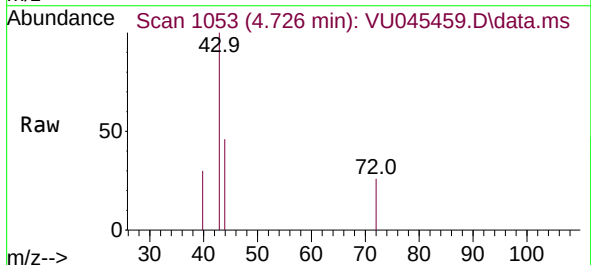



#29

Tetrahydrofuran

Concen: 0.272 ug/l

RT: 5.063 min Scan# 1156

Delta R.T. 0.006 min

Lab File: VU045459.D

Acq: 29 Oct 2021 13:26

Instrument :

MSVOA_U

ClientSampleId :

BP-VPB-RW9-GW-218-220





Tgt Ion: 42 Resp: 383

Ion Ratio Lower Upper

42 100

72 0.0 38.2 57.4#

71 0.0 35.4 53.2#

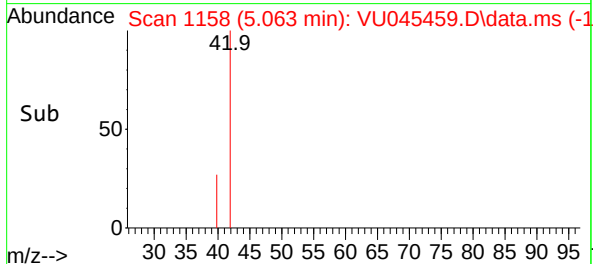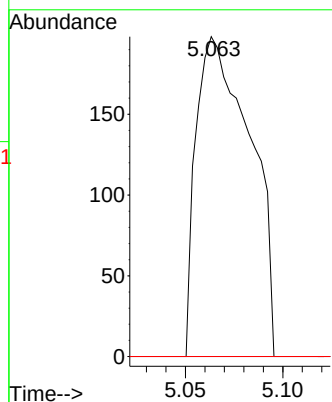

#31

Cyclohexane

Concen: 1.010 ug/l

RT: 5.382 min Scan# 1257

Delta R.T. -0.010 min

Lab File: VU045459.D

Acq: 29 Oct 2021 13:26




Tgt Ion: 56 Resp: 4774


Ion Ratio Lower Upper

56 100

69 188.8 26.4 39.6#

84 146.6 68.4 102.6#


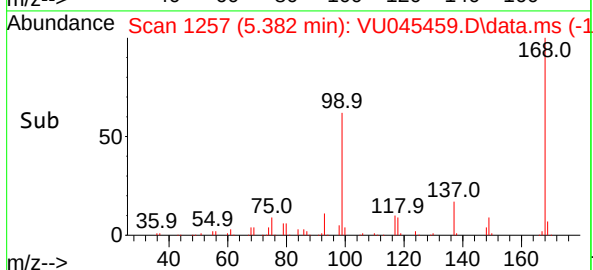






#33
1,2-Dichloroethane-d4
Concen: 51.421 ug/l
RT: 5.706 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion: 65 Resp: 163172
Ion Ratio Lower Upper
65 100
67 52.3 0.0 105.8

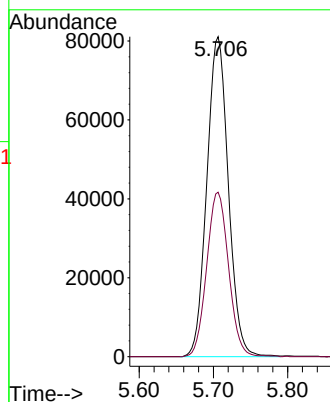

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.253 min Scan# 1528
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 114 Resp: 378889
Ion Ratio Lower Upper
114 100
63 22.5 0.0 45.6
88 16.4 0.0 33.8


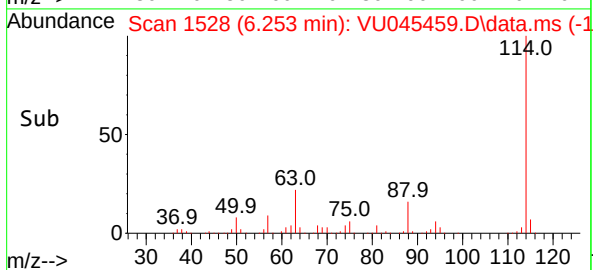
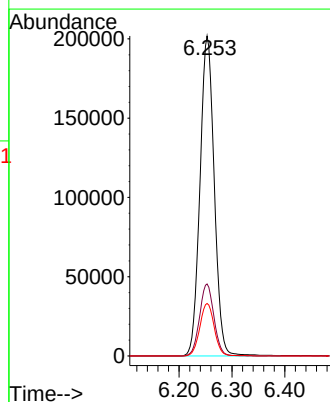
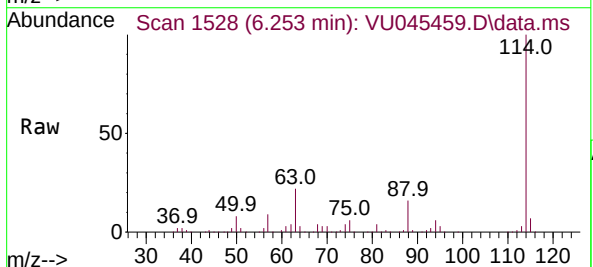




#35
Dibromofluoromethane
Concen: 49.745 ug/l
RT: 5.295 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion:113 Resp: 119843
Ion Ratio Lower Upper
113 100
111 103.1 82.8 124.2
192 18.4 14.8 22.2

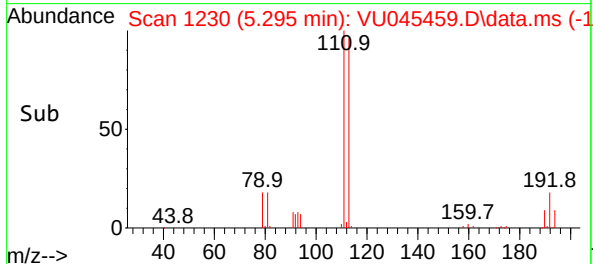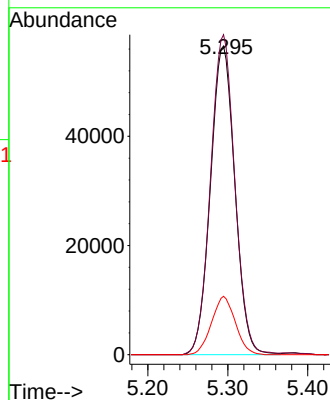

#36
1,1-Dichloropropene
Concen: 4.763 ug/l
RT: 5.378 min Scan# 1256
Delta R.T. -0.151 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26


Tgt Ion: 75 Resp: 17179
Ion Ratio Lower Upper
75 100
110 8.1 16.7 50.0#
77 0.0 25.0 37.4#

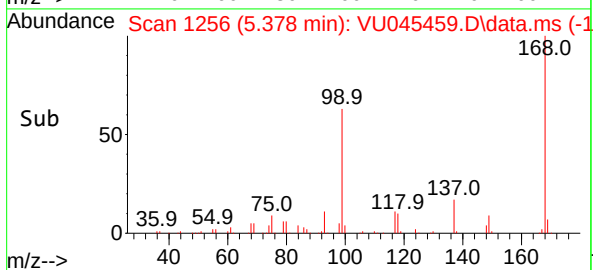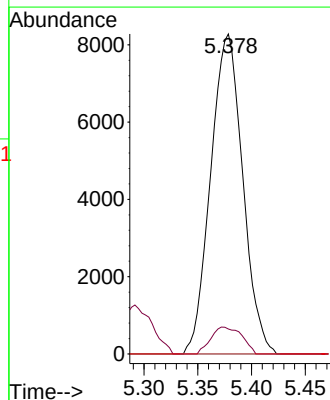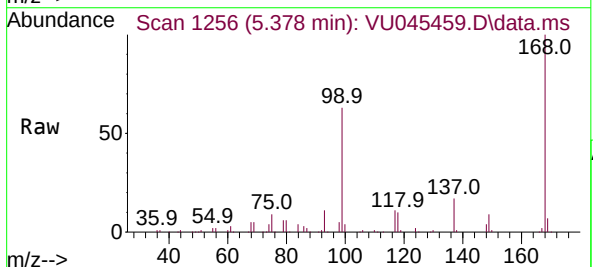






#38
Carbon Tetrachloride
Concen: 6.513 ug/l
RT: 5.378 min Scan# 117
Delta R.T. -0.151 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Instrument : MSVOA_U
ClientSampleId : BP-VPB-RW9-GW-218-220



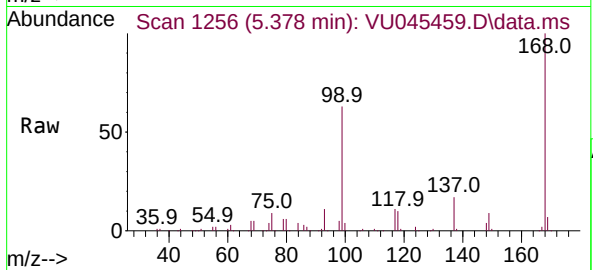



Tgt Ion: 117 Resp: 20487
Ion Ratio Lower Upper
117 100
119 5.2 77.4 116.0#
121 0.0 24.8 37.2#

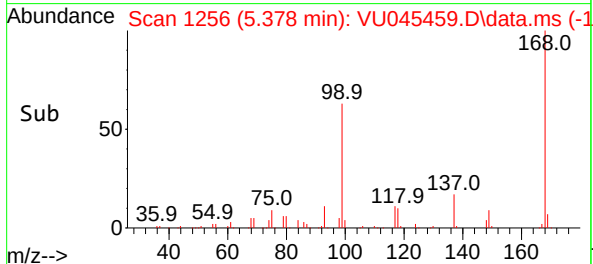

#49
1,4-Dioxane
Concen: 2.169 ug/l
RT: 6.999 min Scan# 1760
Delta R.T. -0.007 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 88 Resp: 172
Ion Ratio Lower Upper
88 100
43 0.0 0.0 0.0
58 75.6 58.7 88.1


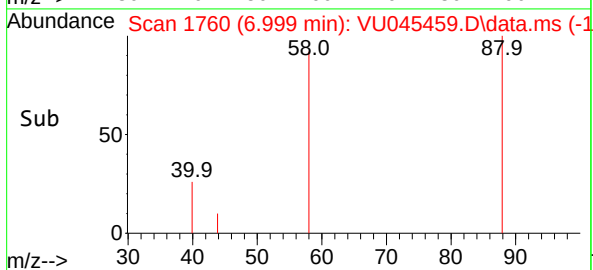

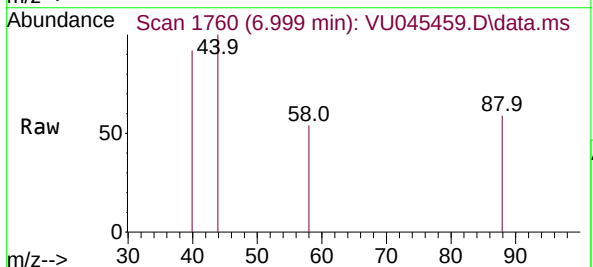




#50
Toluene-d8
Concen: 51.252 ug/l
RT: 7.902 min Scan# 2041
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument : MSVOA_U
ClientSampleId : BP-VPB-RW9-GW-218-220


Tgt Ion: 98 Resp: 484187
Ion Ratio Lower Upper
98 100
100 65.3 52.5 78.7

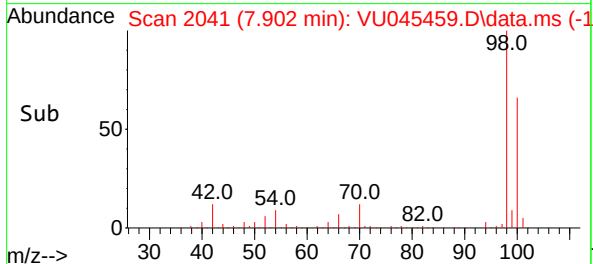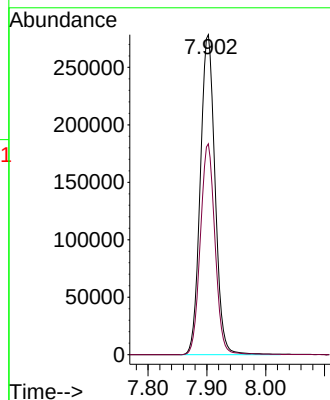

#51
4-Methyl-2-Pentanone
Concen: 0.306 ug/l
RT: 7.796 min Scan# 2008
Delta R.T. 0.003 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 43 Resp: 1303
Ion Ratio Lower Upper
43 100
58 38.1 33.8 50.8

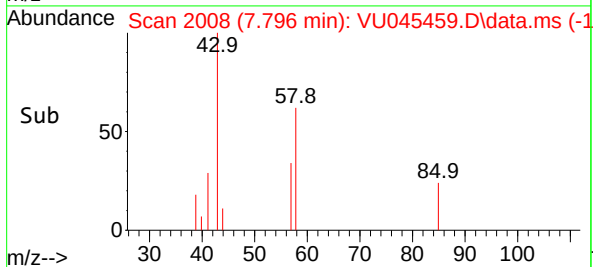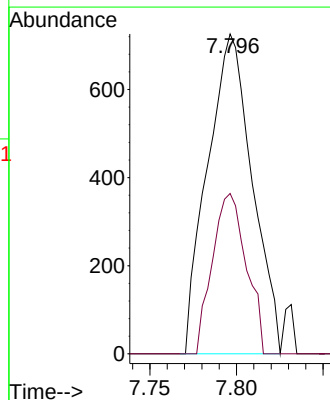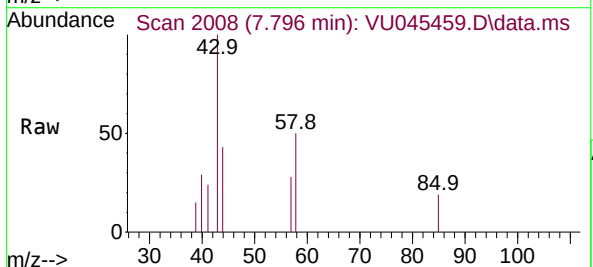



#56

Ethyl methacrylate

Concen: 1.670 ug/l

RT: 8.340 min Scan# 2176

Delta R.T. 0.003 min

Lab File: VU045459.D

Acq: 29 Oct 2021 13:26

Instrument :

MSVOA_U

ClientSampleId :

BP-VPB-RW9-GW-218-220





Tgt Ion: 69 Resp: 149

Ion Ratio Lower Upper

69 100

41 77.9 51.0 76.4#

39 26.8 26.6 39.8

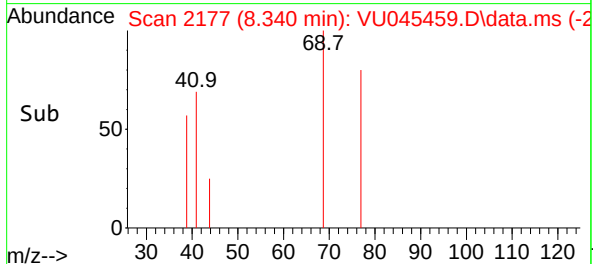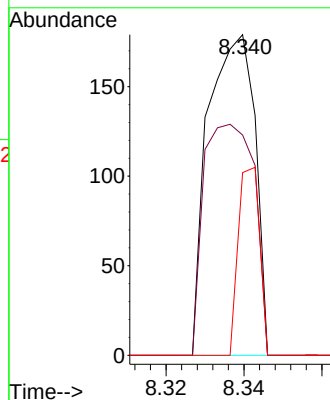

#59

2-Hexanone

Concen: 0.451 ug/l

RT: 8.690 min Scan# 2286

Delta R.T. 0.003 min

Lab File: VU045459.D




Acq: 29 Oct 2021 13:26


Tgt Ion: 43 Resp: 1487

Ion Ratio Lower Upper

43 100

58 54.7 29.5 88.6


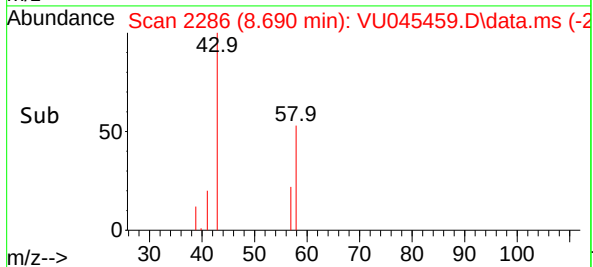
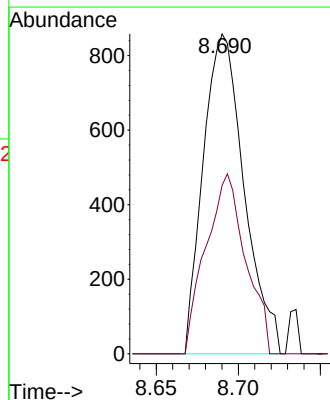
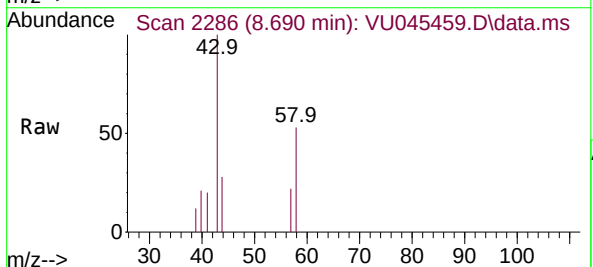




#62
4-Bromofluorobenzene
Concen: 50.234 ug/l
RT: 10.635 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument : MSVOA_U
ClientSampleId : BP-VPB-RW9-GW-218-220


Tgt Ion: 95 Resp: 180840
Ion Ratio Lower Upper
95 100
174 71.2 0.0 141.8
176 67.0 0.0 138.2

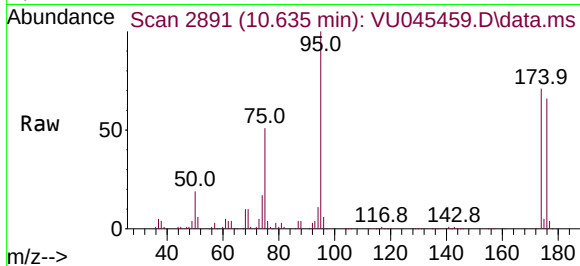

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 117 Resp: 364747
Ion Ratio Lower Upper
117 100
82 59.8 47.8 71.8
119 32.0 25.8 38.8


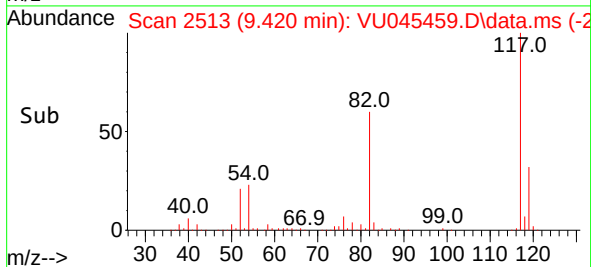

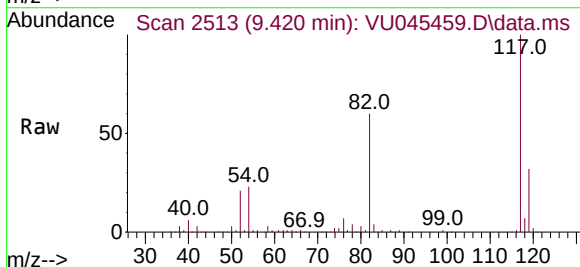




#68
m/p-Xylenes
Concen: 0.268 ug/l
RT: 9.696 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion:106 Resp: 1280
Ion Ratio Lower Upper
106 100
91 198.3 164.7 247.1

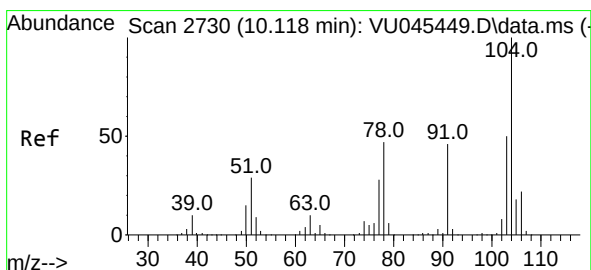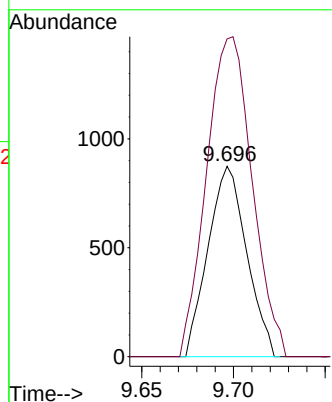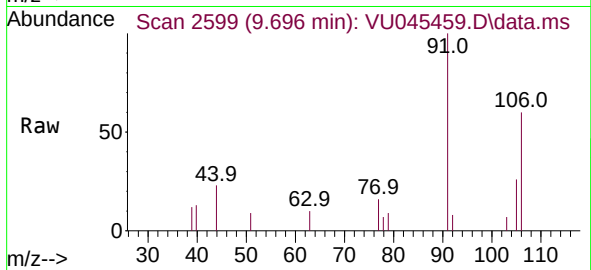

#70
Styrene
Concen: 1.102 ug/l
RT: 10.118 min Scan# 2730
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion:104 Resp: 1107
Ion Ratio Lower Upper
104 100
78 45.3 41.8 62.6
103 50.9 43.8 65.6


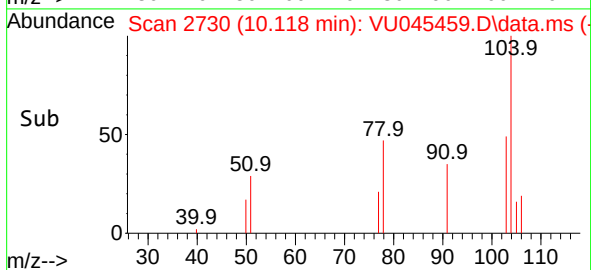
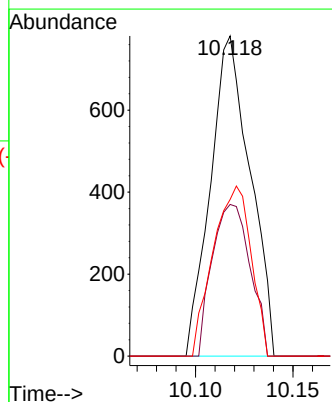
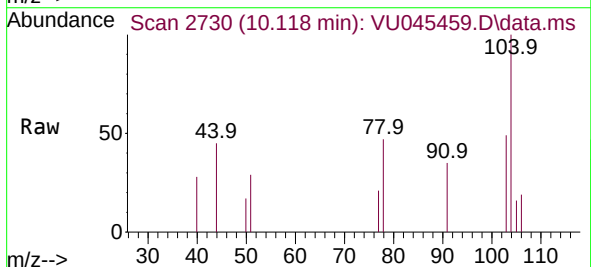




#71
Bromoform
Concen: 2.029 ug/l
RT: 10.295 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion:173 Resp: 96
Ion Ratio Lower Upper
173 100
175 0.0 24.1 72.2#
254 0.0 0.0 0.0

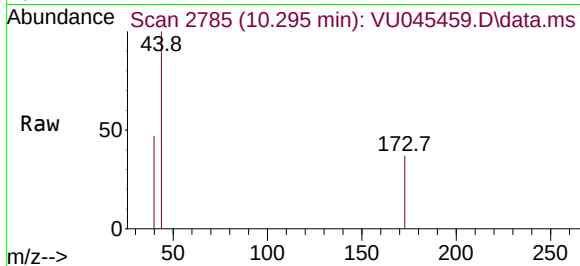

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.815 min Scan# 3258
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion:152 Resp: 175516
Ion Ratio Lower Upper
152 100
115 61.5 42.7 128.1
150 156.2 0.0 346.8


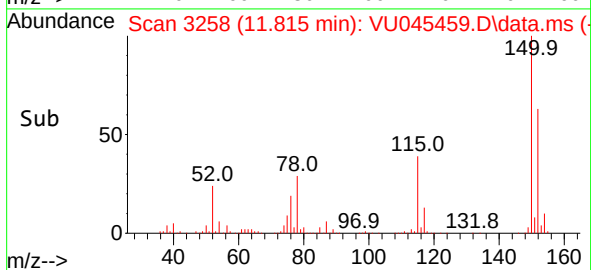




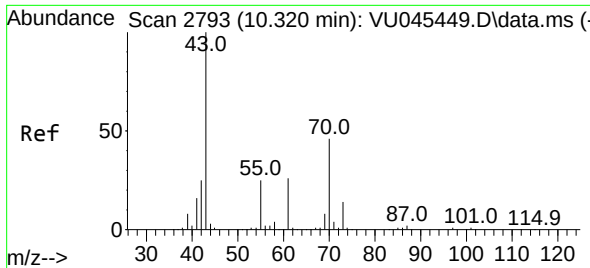

#74
N-amy1 acetate
Concen: 1.210 ug/l
RT: 10.320 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion:	43	Resp:	347
Ion	Ratio	Lower	Upper
43	100		
70	26.8	36.9	55.3#
55	6.1	20.6	31.0#
61	0.0	20.5	30.7#

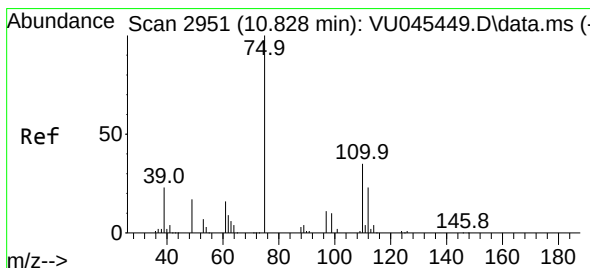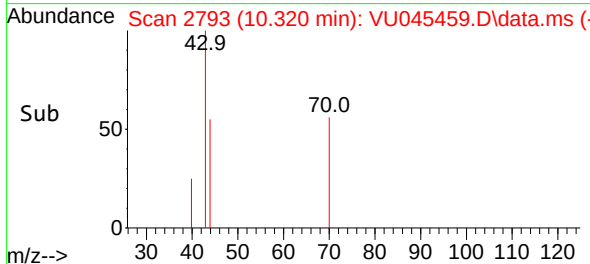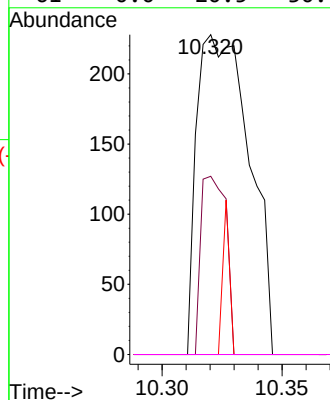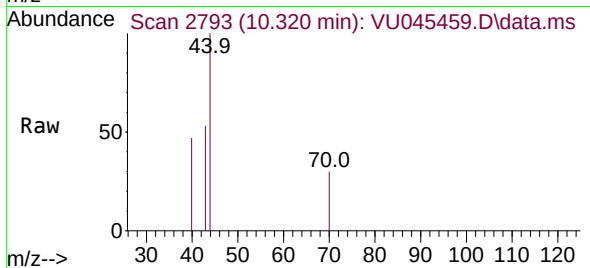

#76
1,2,3-Trichloropropane
Concen: 19.925 ug/l
RT: 10.635 min Scan# 2891
Delta R.T. -0.193 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion:	75	Resp:	93177
Ion	Ratio	Lower	Upper
75	100		
77	1.1	17.1	51.3#


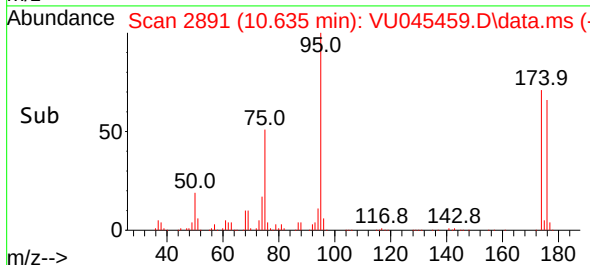
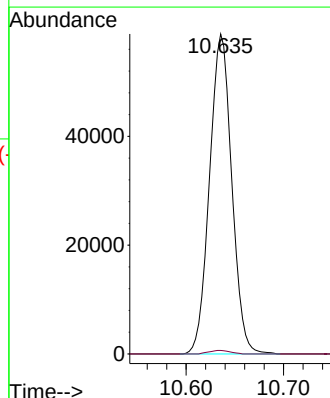
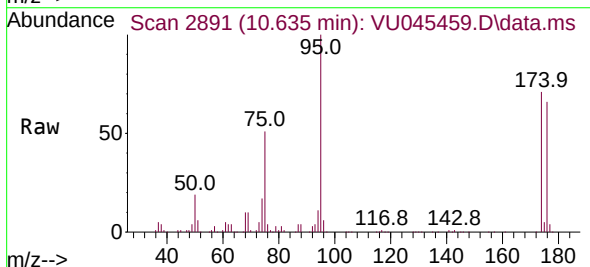




#81
trans-1,4-Dichloro-2-butene
Concen: 55.353 ug/l
RT: 10.635 min Scan# 2864
Delta R.T. 0.086 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion: 75 Resp: 93177
Ion Ratio Lower Upper
75 100
53 0.0 76.2 114.4#
89 0.0 34.0 51.0#

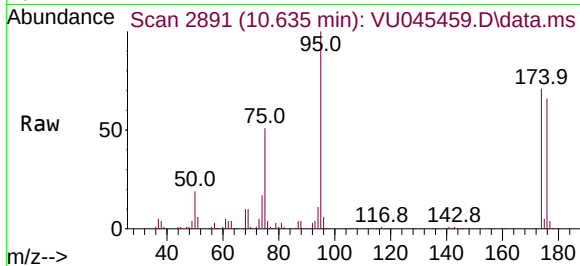

#82
4-Chlorotoluene
Concen: 0.235 ug/l
RT: 11.098 min Scan# 3035
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 91 Resp: 2304
Ion Ratio Lower Upper
91 100
126 22.0 13.8 41.4


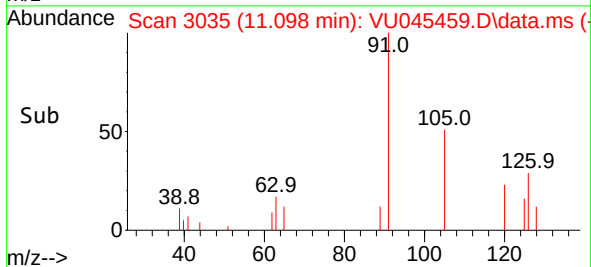

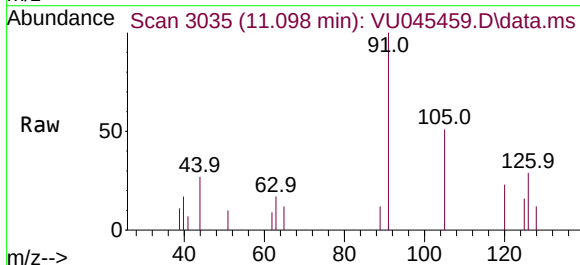




#86
p-Isopropyltoluene
Concen: 0.347 ug/l
RT: 11.796 min Scan# 31
Delta R.T. 0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion:	119	Resp:	1789
Ion	Ratio	Lower	Upper
119	100		
134	24.5	12.7	38.1
91	52.9	12.2	36.4#

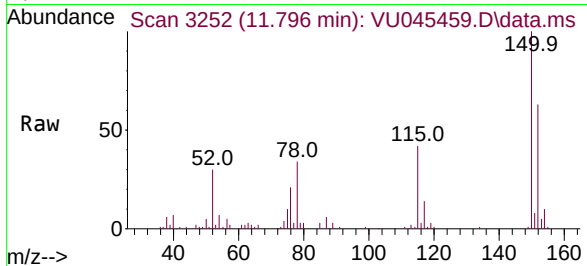

#87
1,3-Dichlorobenzene
Concen: 0.305 ug/l
RT: 11.748 min Scan# 3237
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion:	146	Resp:	1664
Ion	Ratio	Lower	Upper
146	100		
111	36.3	21.3	63.9
148	68.0	31.7	95.1


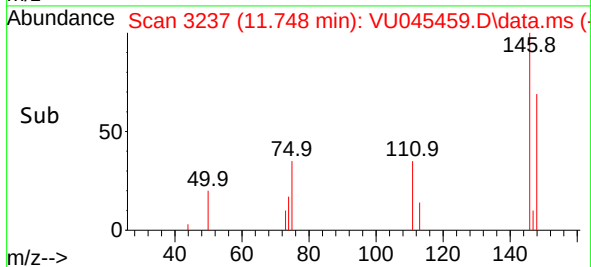

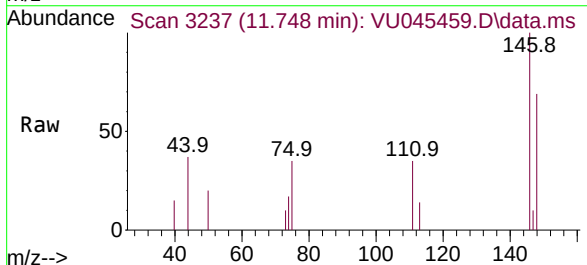




#88
1,4-Dichlorobenzene
Concen: 0.299 ug/l
RT: 11.748 min Scan# 31
Delta R.T. -0.090 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion:146 Resp: 1664
Ion Ratio Lower Upper
146 100
111 36.3 20.6 61.9
148 68.0 31.9 95.7

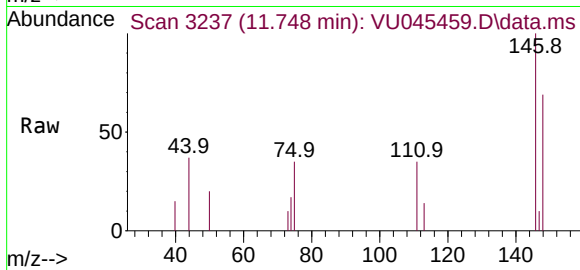

#89
n-Butylbenzene
Concen: 1.211 ug/l
RT: 12.214 min Scan# 3382
Delta R.T. 0.003 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion: 91 Resp: 3038
Ion Ratio Lower Upper
91 100
92 52.7 27.1 81.2
134 21.3 11.8 35.4


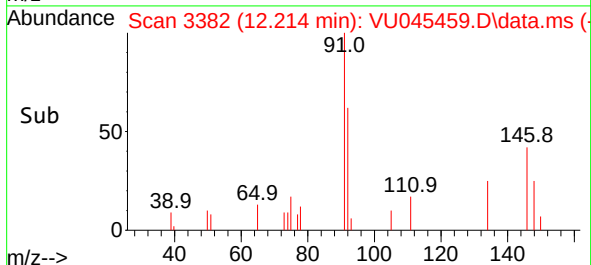

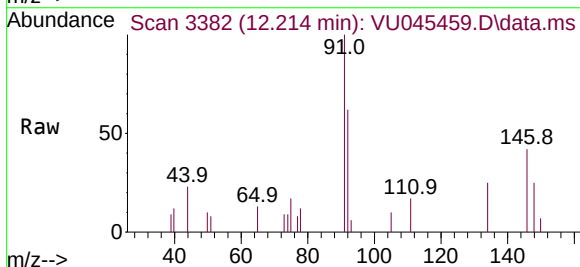




#91
1,2-Dichlorobenzene
Concen: 0.229 ug/l
RT: 12.214 min Scan# 311
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220


Tgt Ion:146 Resp: 1249
Ion Ratio Lower Upper
146 100
111 45.6 21.9 65.5
148 57.6 32.1 96.3

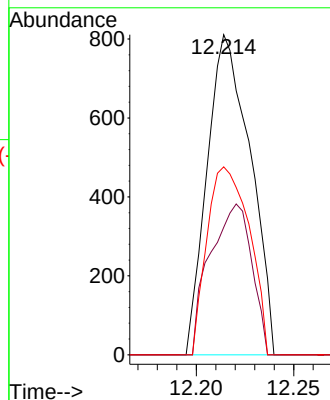

#93
1,2,4-Trichlorobenzene
Concen: 0.570 ug/l
RT: 13.844 min Scan# 3889
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26


Tgt Ion:180 Resp: 2081
Ion Ratio Lower Upper
180 100
182 90.0 47.0 141.2
145 27.5 15.6 46.7

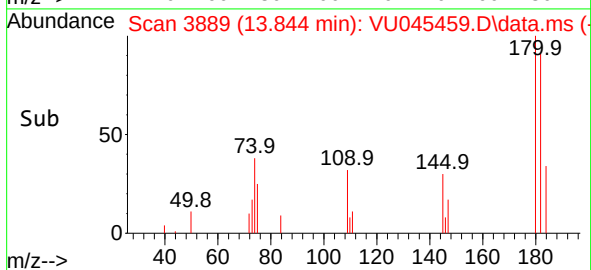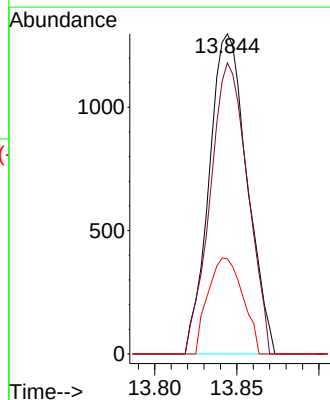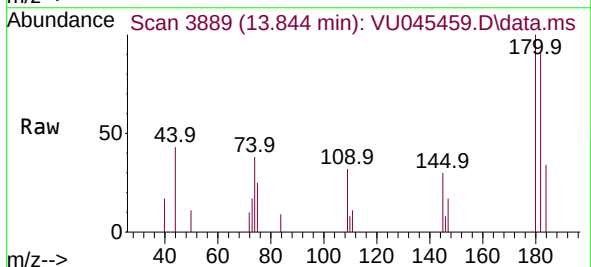






#94
Hexachlorobutadiene
Concen: 0.396 ug/l
RT: 14.024 min Scan# 3945
Delta R.T. -0.000 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-218-220



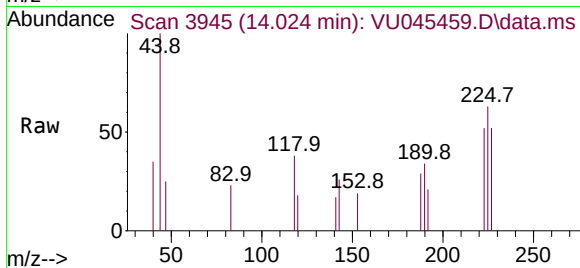



Tgt Ion	Ratio	Lower	Upper
225	100		
223	70.9	32.0	96.2
227	72.2	31.1	93.5

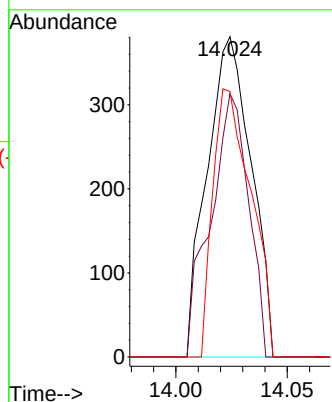

#95
Naphthalene
Concen: 0.523 ug/l
RT: 14.092 min Scan# 3966
Delta R.T. 0.003 min
Lab File: VU045459.D
Acq: 29 Oct 2021 13:26

Tgt Ion	Ratio	Lower	Upper
128	100		
127	12.5	10.6	15.8
129	8.6	8.6	13.0

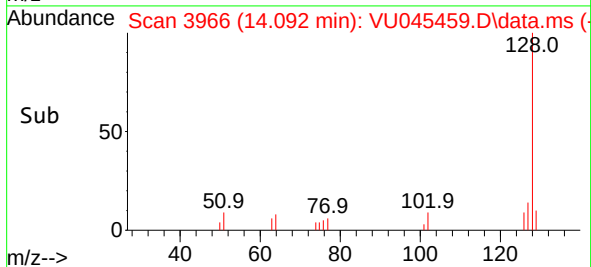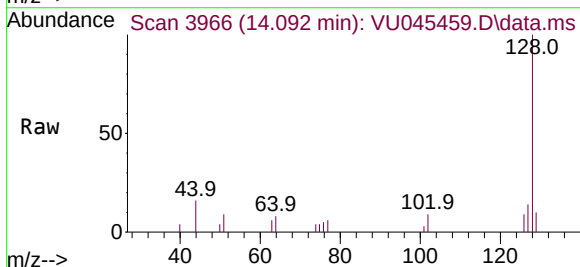



#96

1,2,3-Trichlorobenzene

Concen: 0.552 ug/l

RT: 14.333 min Scan# 4041

Delta R.T. -0.000 min

Lab File: VU045459.D


Acq: 29 Oct 2021 13:26

Instrument :

MSVOA_U

ClientSampleId :

BP-VPB-RW9-GW-218-220

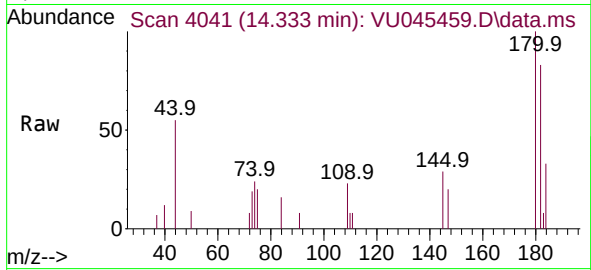

Tgt Ion:180 Resp: 2031

Ion Ratio Lower Upper

180 100

182 90.4 47.7 143.1

145 33.5 16.7 50.0

