


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103018\
Data File : VU027864.D
Acq On : 30 Oct 2018 10:08
Operator : MD/SY
Sample : BFB51
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB51

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR103018WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Oct 31 02:11:32 2018

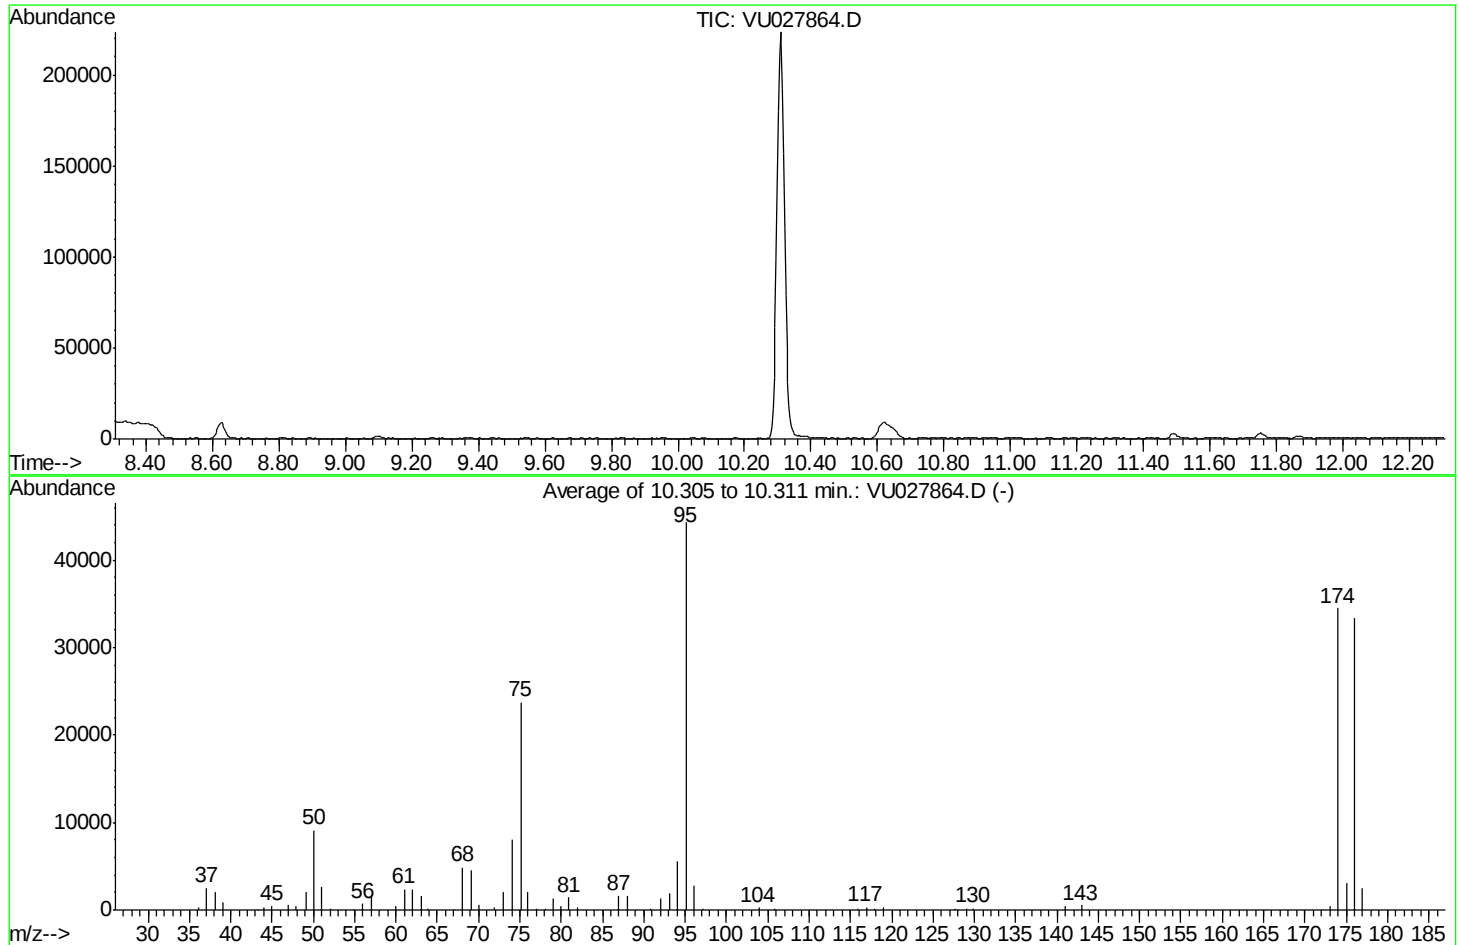

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	9117	PASS
75	95	30	80	53.5	23714	PASS
95	95	100	100	100.0	44330	PASS
96	95	5	9	6.3	2779	PASS
173	174	0.00	2	1.2	419	PASS
174	95	50	120	77.9	34520	PASS
175	174	5	9	8.9	3077	PASS
176	174	95	101	96.5	33328	PASS
177	176	5	9	7.5	2498	PASS

m/z	Abundance
44.00	321.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.10	326.0
37.10	2672.0
38.10	2125.0
39.00	847.0
44.00	695.0
45.00	436.0
47.00	488.0
47.90	420.0
49.00	1933.0
50.10	8762.0
51.00	2613.0
52.00	151.0
56.00	792.0
57.00	1444.0
60.00	476.0
61.00	2357.0
62.00	2299.0
63.10	1488.0
63.90	194.0
67.00	121.0
68.10	4678.0
69.10	4614.0
70.00	487.0
71.90	373.0
73.00	2040.0
74.10	7940.0
75.10	23248.0
76.00	2049.0
77.10	228.0
78.00	148.0
78.90	1322.0
80.00	362.0
80.90	1321.0
81.90	263.0
87.00	1582.0
88.00	1675.0
90.80	155.0
92.10	1246.0
93.10	2016.0
94.00	5313.0
95.10	43048.0
96.10	2659.0
103.90	269.0
105.80	163.0
115.90	188.0
116.90	306.0
117.90	198.0
119.00	266.0
127.70	146.0
130.00	146.0
141.00	493.0
142.90	506.0
174.00	32704.0
175.00	2985.0
176.00	31696.0
177.00	2417.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	363.0
37.10	2661.0
38.10	2156.0
39.10	832.0
44.00	704.0
45.00	473.0
47.00	628.0
47.90	394.0
49.00	2037.0
50.10	9390.0
51.00	2601.0
52.10	157.0
56.00	715.0
57.00	1475.0
60.00	499.0
61.00	2421.0
62.00	2363.0
63.00	1581.0
63.90	176.0
68.10	4985.0
69.10	4681.0
70.00	557.0
71.90	306.0
73.00	2101.0
74.10	8237.0
75.10	24536.0
76.00	2067.0
77.10	183.0
78.10	138.0
79.00	1378.0
80.00	459.0
80.90	1471.0
81.90	266.0
87.00	1666.0
88.00	1603.0
90.80	175.0
92.00	1396.0
93.10	2028.0
94.10	5764.0
95.10	45608.0
96.10	2855.0
97.10	115.0
103.90	276.0
105.80	213.0
115.90	195.0
116.90	348.0
117.90	218.0
119.00	266.0
127.70	120.0
129.00	125.0
129.90	166.0
141.00	505.0
143.00	562.0
173.00	703.0
174.00	35544.0
175.00	3194.0
176.00	34296.0
177.00	2635.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	405.0
37.00	2346.0
38.10	1958.0
39.10	757.0
43.20	122.0
44.00	659.0
45.00	441.0
47.00	689.0
48.00	342.0
49.10	1976.0
50.10	9201.0
51.10	2494.0
52.10	153.0
54.90	106.0
56.00	618.0
57.00	1327.0
60.00	480.0
61.10	2343.0
62.00	2242.0
63.00	1622.0
63.90	144.0
68.00	4850.0
69.10	4376.0
70.00	541.0
71.90	202.0
73.00	2032.0
74.10	7877.0
75.10	23360.0
76.00	1994.0
77.00	171.0
78.00	137.0
79.00	1325.0
80.00	464.0
80.90	1425.0
81.90	268.0
87.00	1591.0
88.10	1456.0
90.90	203.0
92.00	1388.0
93.10	1796.0
94.10	5485.0
95.10	44336.0
96.10	2824.0
97.10	122.0
103.90	203.0
105.80	229.0
115.90	177.0
116.90	313.0
117.90	191.0
119.00	225.0
128.00	113.0
129.00	122.0
129.80	182.0
141.00	492.0
143.00	558.0
171.90	102.0
173.00	556.0
174.00	35312.0
175.00	3054.0
176.00	33992.0
177.00	2442.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51