

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU103019\
Data File : VU035550.D
Acq On : 30 Oct 2019 09:59
Operator : JC/SP
Sample : VU1030WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1030WBL01

Quant Time: Oct 31 01:19:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Oct 30 07:13:39 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	6.16	96	66294	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.67	95	19608	0.82	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.00%	
68) 1,2-Dichlorobenzene-d4	12.22	152	19190	0.76	ug/l	0.00
Spiked Amount 1.000			Recovery	=	76.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU103019\
Data File : VU035550.D
Acq On : 30 Oct 2019 09:59
Operator : JC/SP
Sample : VU1030WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1030WBL01

Quant Time: Oct 31 01:19:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Oct 30 07:13:39 2019
Response via : Initial Calibration

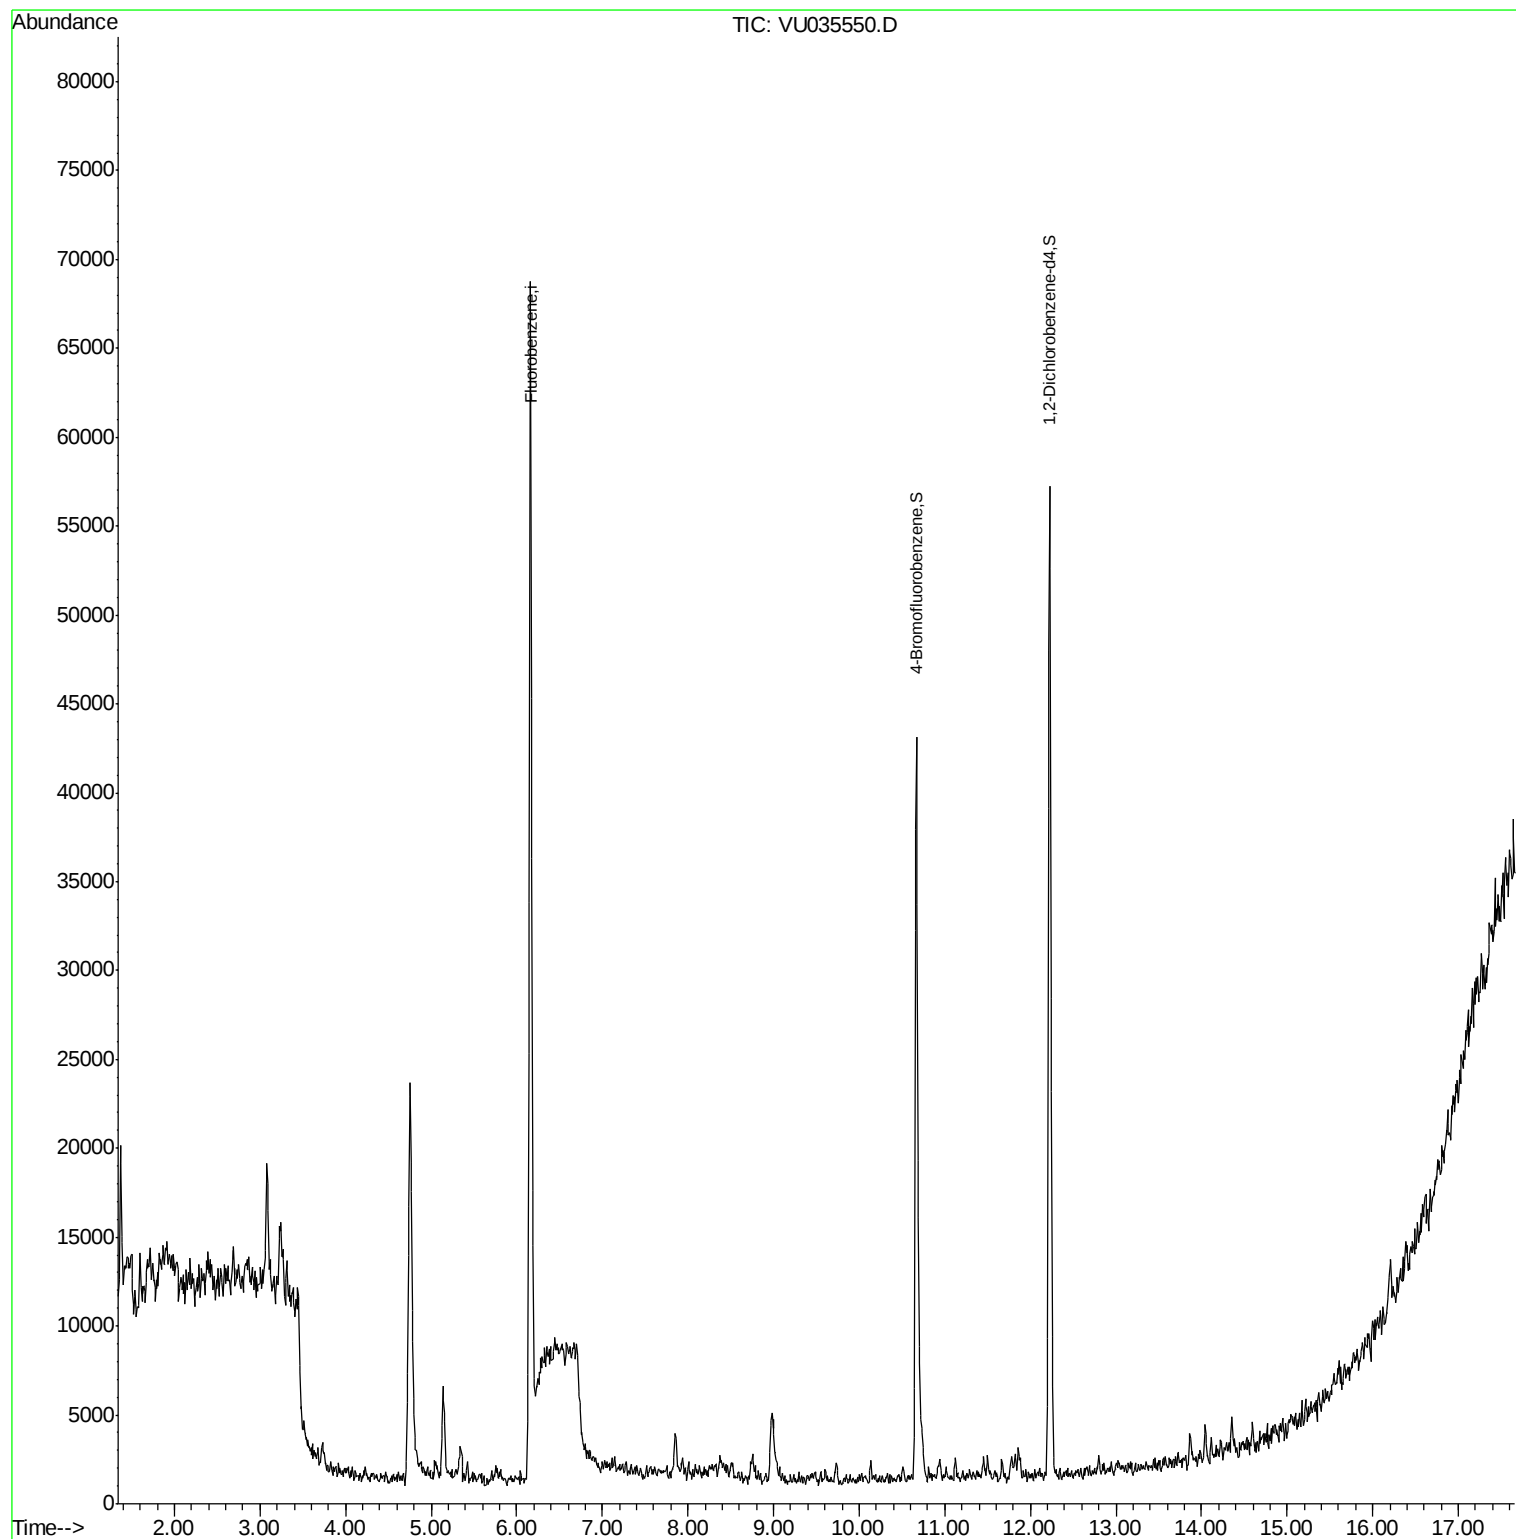

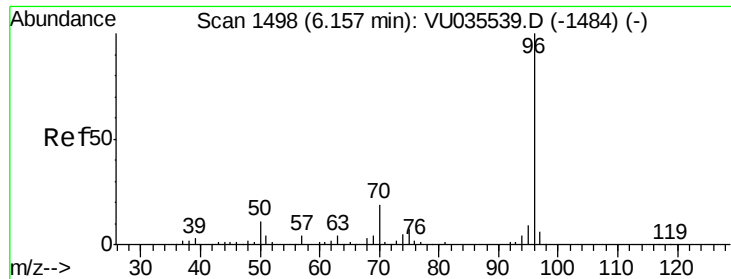

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.16 min Scan# 1499

Delta R.T. 0.00 min

Lab File: VU035550.D

Acq: 30 Oct 2019 09:59

Instrument :

MSVOA_U

ClientSampleId :

VU1030WBL01

Tgt Ion: 96 Resp: 66294


Ion Ratio Lower Upper

96 100

70 19.7 15.8 23.8

95 8.7 7.4 11.2

97 6.6 0.0 0.0#



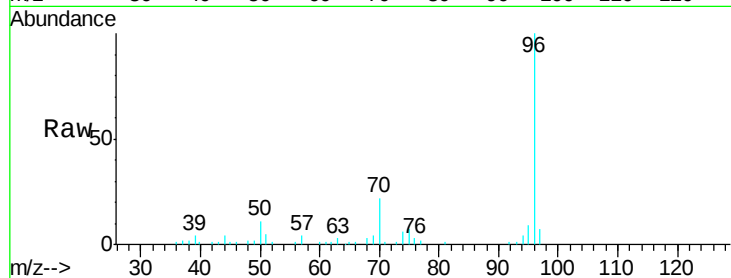


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

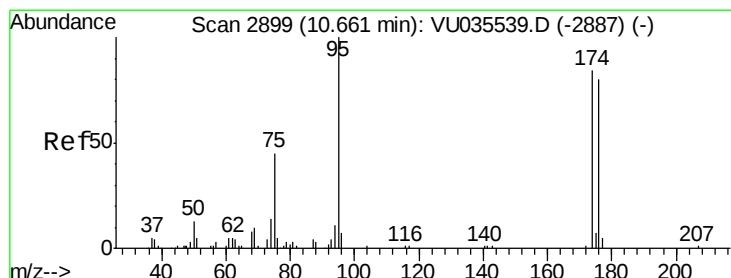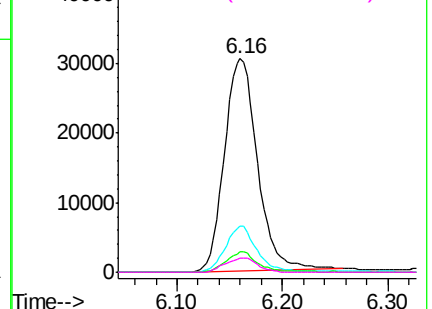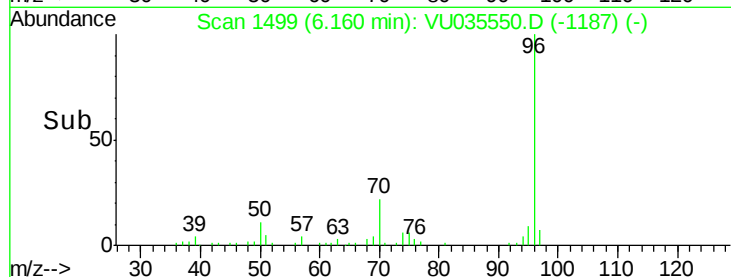

#57

4-Bromofluorobenzene

Concen: 0.822 ug/l

RT: 10.67 min Scan# 2901

Delta R.T. 0.01 min

Lab File: VU035550.D

Acq: 30 Oct 2019 09:59


Tgt Ion: 95 Resp: 19608

Ion Ratio Lower Upper

95 100

174 91.4 70.2 105.4



176 84.4 67.7 101.5

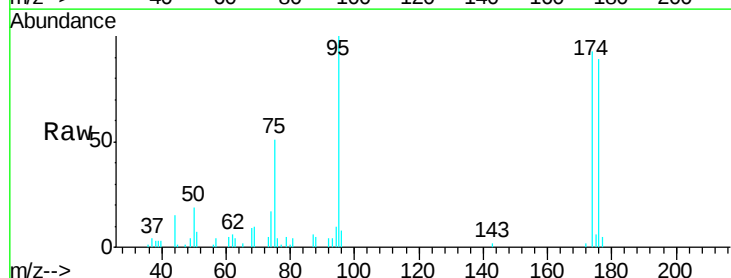


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

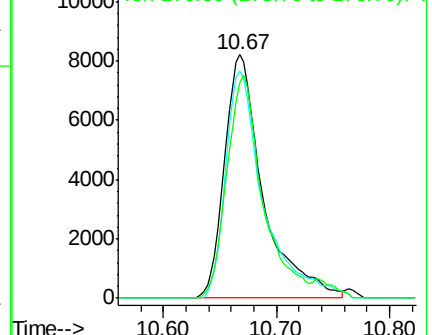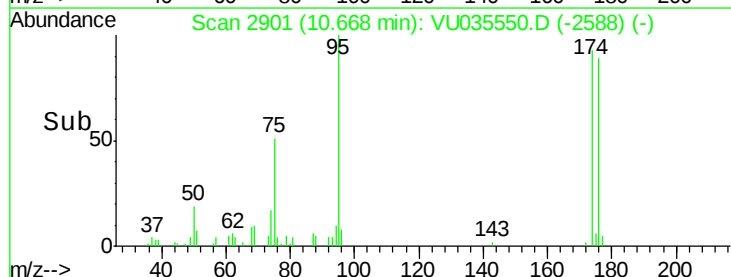

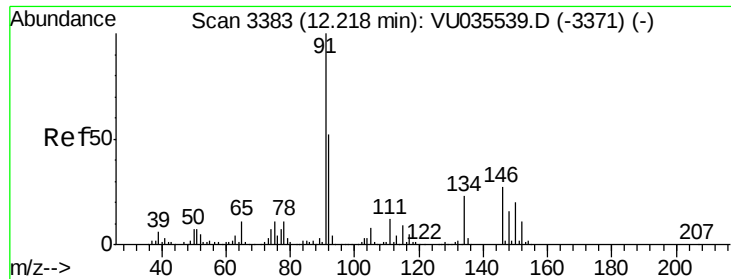

#68

1,2-Dichlorobenzene-d4

Concen: 0.757 ug/l

RT: 12.22 min Scan# 3385

Delta R.T. 0.01 min

Lab File: VU035550.D


Acq: 30 Oct 2019 09:59

Instrument :

MSVOA_U

ClientSampleId :

VU1030WBL01

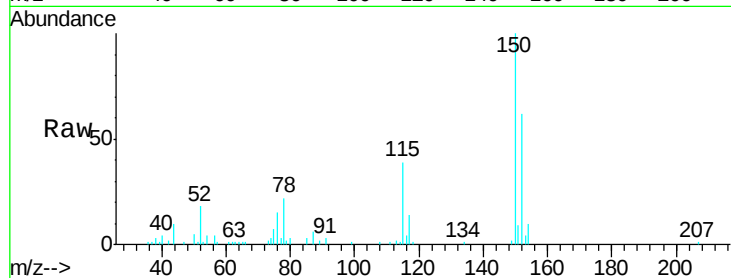

Tgt Ion:152 Resp: 19190

Ion Ratio Lower Upper

152 100

115 64.1 0.0 250.6

150 158.2 0.0 656.8

