

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103019\
 Data File : VU035550.D
 Acq On : 30 Oct 2019 09:59
 Operator : JC/SP
 Sample : VU1030WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1030WBL01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.729	735	743	748	rBV8	1145	1824	1.21%	0.388%
2	4.755	1043	1062	1082	rBV2	22696	68736	45.50%	14.605%
3	5.141	1171	1182	1198	rBV4	5009	10426	6.90%	2.215%
4	5.343	1237	1245	1248	rBV6	1641	2425	1.61%	0.515%
5	5.424	1263	1270	1276	rVB4	1264	1941	1.28%	0.412%
6	6.160	1483	1499	1518	rBV	67423	151066	100.00%	32.098%
7	7.854	2018	2026	2032	rBV8	1823	2992	1.98%	0.636%
8	8.980	2364	2376	2380	rBV7	3855	7619	5.04%	1.619%
9	10.668	2889	2901	2933	rBV	41780	95253	63.05%	20.239%
10	11.456	3137	3146	3149	rBV4	1203	1561	1.03%	0.332%
11	11.777	3237	3246	3248	rBV3	1215	1650	1.09%	0.351%
12	12.224	3373	3385	3402	rBV2	55590	116288	76.98%	24.709%
13	13.861	3889	3894	3896	rBV4	1921	1654	1.09%	0.351%
14	14.041	3944	3950	3958	rBV5	1875	2369	1.57%	0.503%
15	14.118	3966	3974	3979	rBV4	1533	2176	1.44%	0.462%
16	14.356	4041	4048	4054	rBV8	2011	2655	1.76%	0.564%


Sum of corrected areas: 470635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103019\
Data File : VU035550.D
Acq On : 30 Oct 2019 09:59
Operator : JC/SP
Sample : VU1030WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1030WBL01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

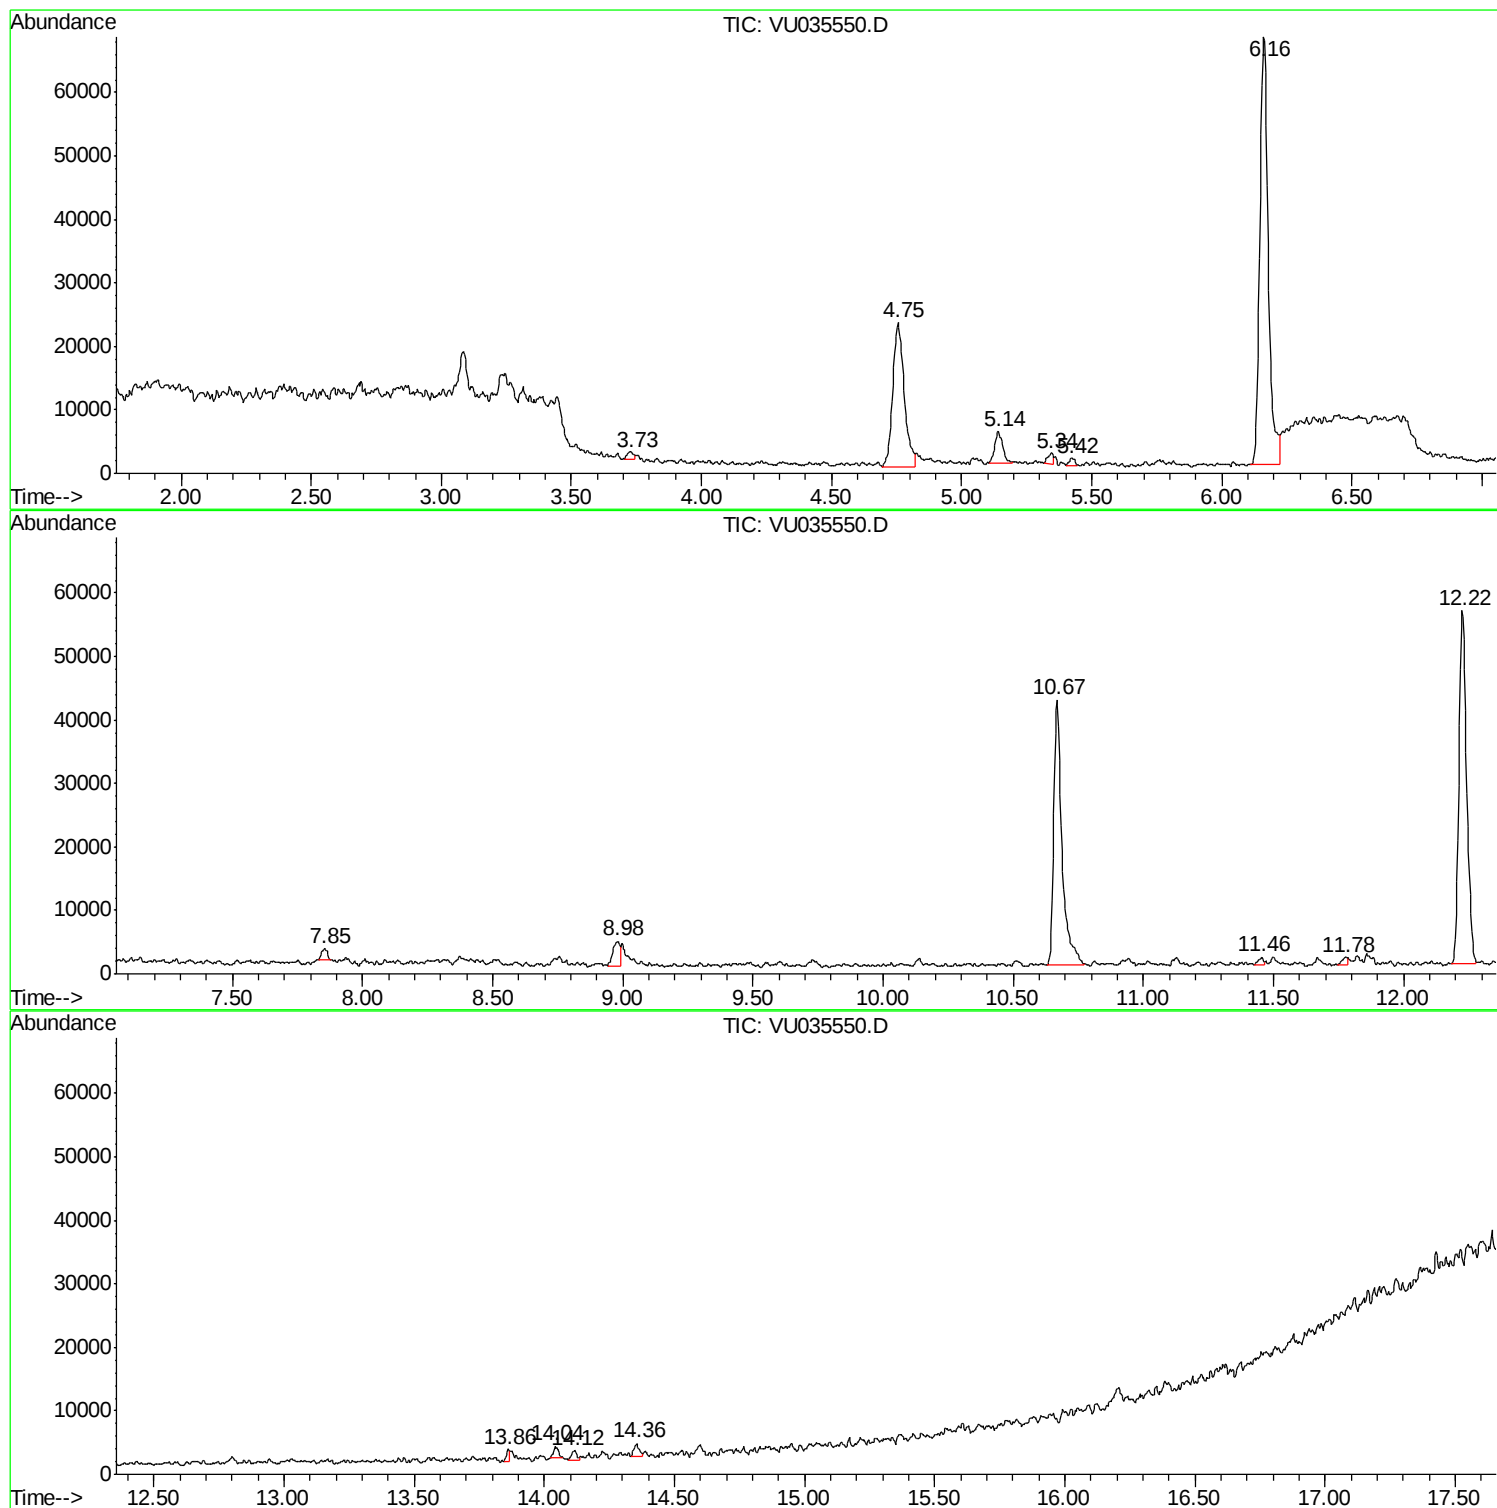

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103019\
Data File : VU035550.D
Acq On : 30 Oct 2019 09:59
Operator : JC/SP
Sample : VU1030WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1030WBL01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103019\
Data File : VU035550.D
Acq On : 30 Oct 2019 09:59
Operator : JC/SP
Sample : VU1030WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1030WBL01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc