


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103019\
Data File : VU035548.D
Acq On : 30 Oct 2019 07:42
Operator : JC/SP
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102919DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Oct 31 01:39:57 2019

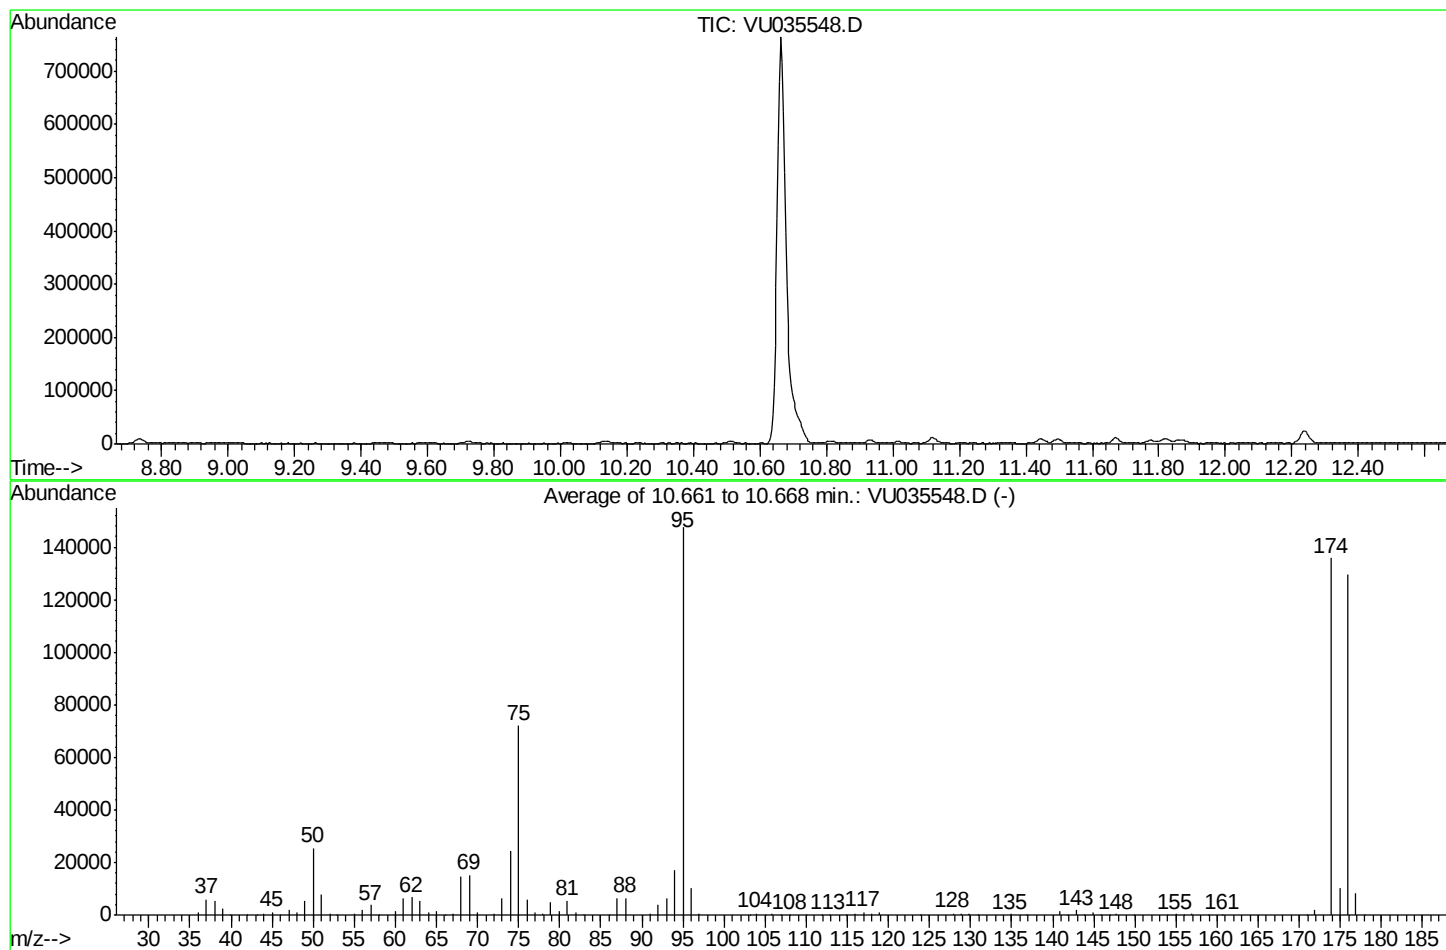

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	25549	PASS
75	95	30	60	48.8	71960	PASS
95	95	100	100	100.0	147498	PASS
96	95	5	9	7.1	10423	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.0	135680	PASS
175	174	5	9	7.6	10278	PASS
176	174	95	101	95.5	129629	PASS
177	176	5	9	6.5	8436	PASS