


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
Data File : VU041027.D
Acq On : 29 Oct 2020 20:36
Operator : SY/MD
Sample : L4558-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BQ2

Manual Integrations
APPROVED

MMDadoda
11/2/2020 4:59:46 PM

Quant Time: Oct 30 09:17:59 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 30 08:06:28 2020
Response via : Initial Calibration

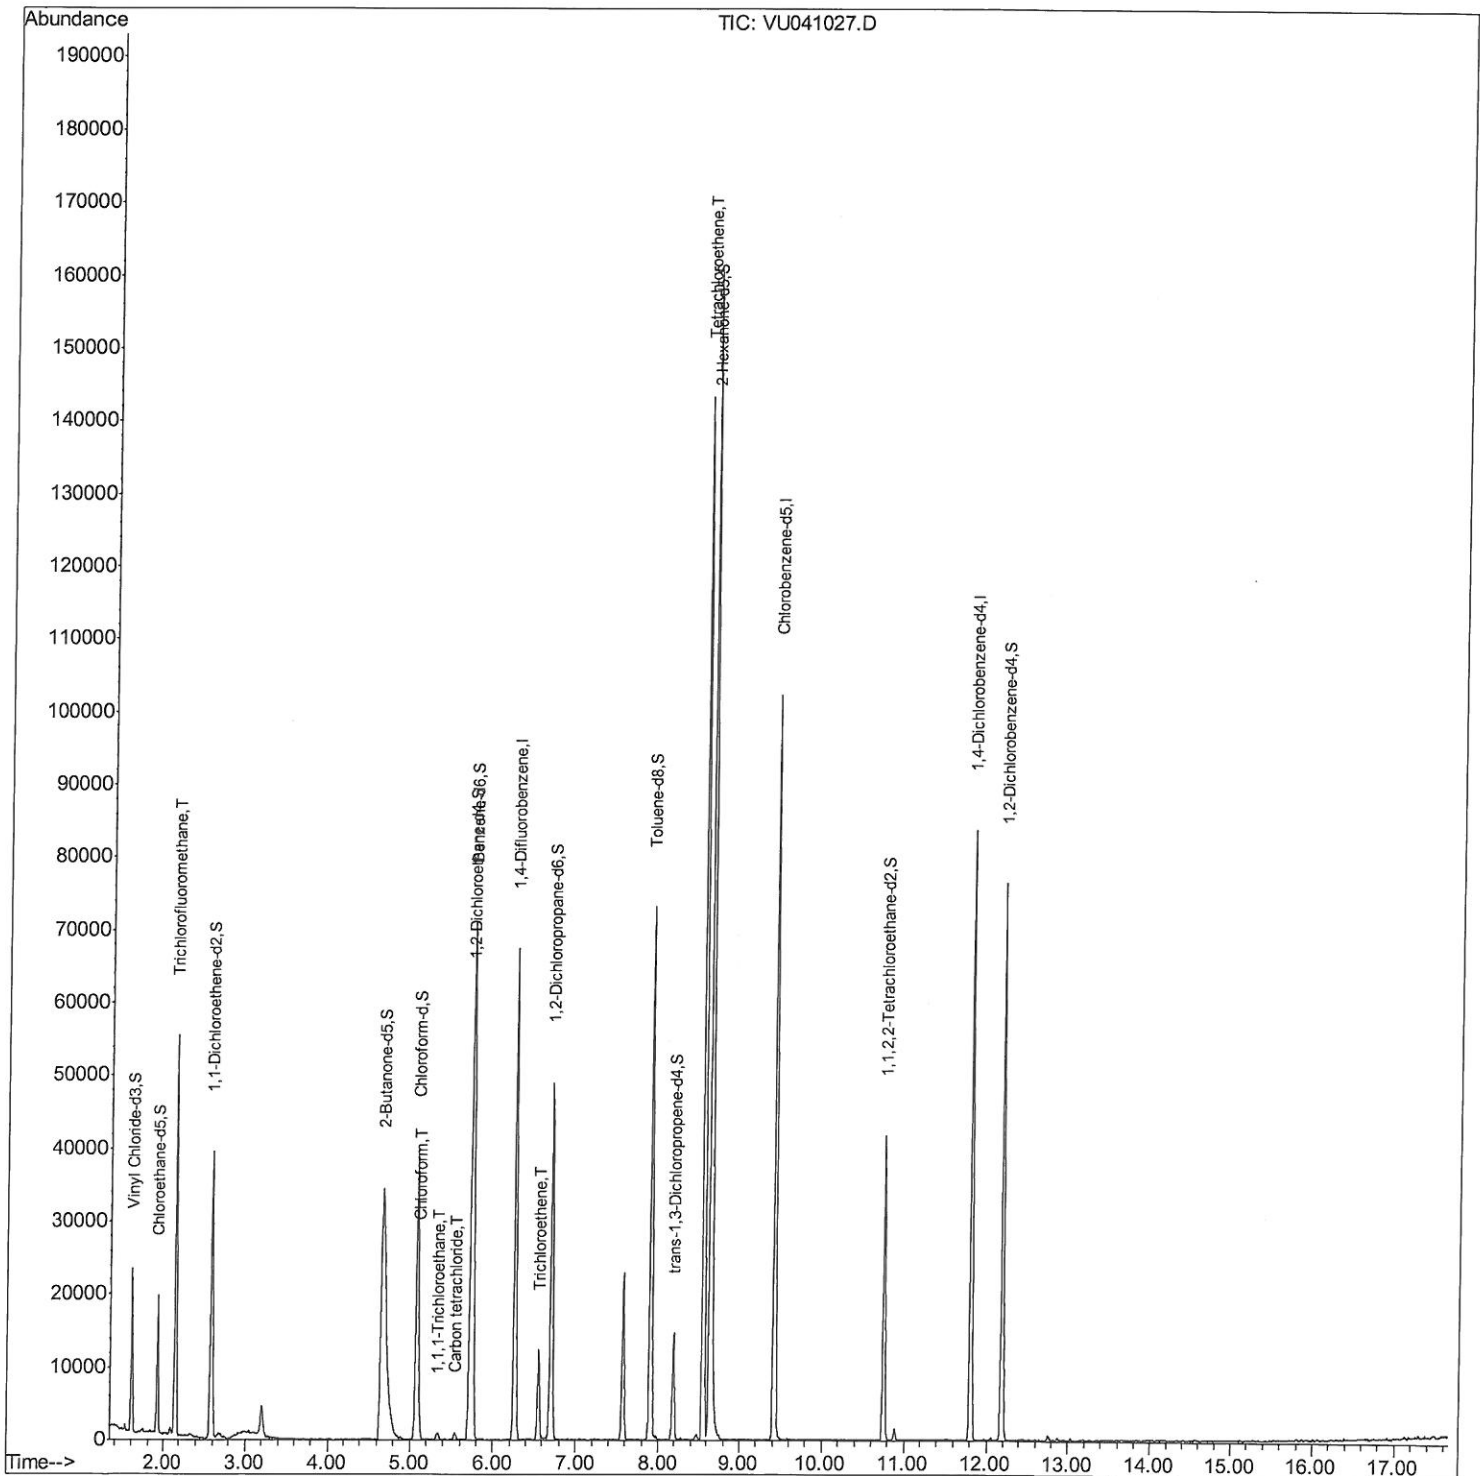

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
Data File : VU041027.D
Acq On : 29 Oct 2020 20:36
Operator : SY/MD
Sample : L4558-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BQ2

Manual Integrations
APPROVED

MMDadoda
11/2/2020 4:59:46 PM

Quant Time: Oct 30 09:17:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 30 08:06:28 2020
Response via : Initial Calibration

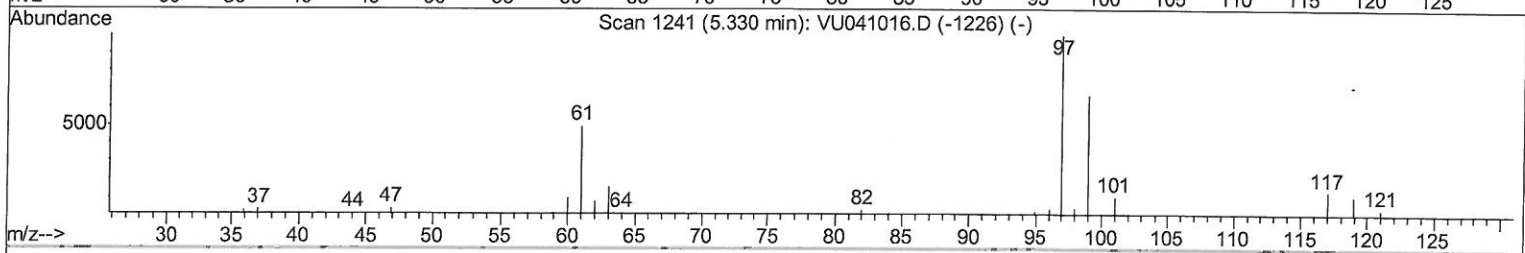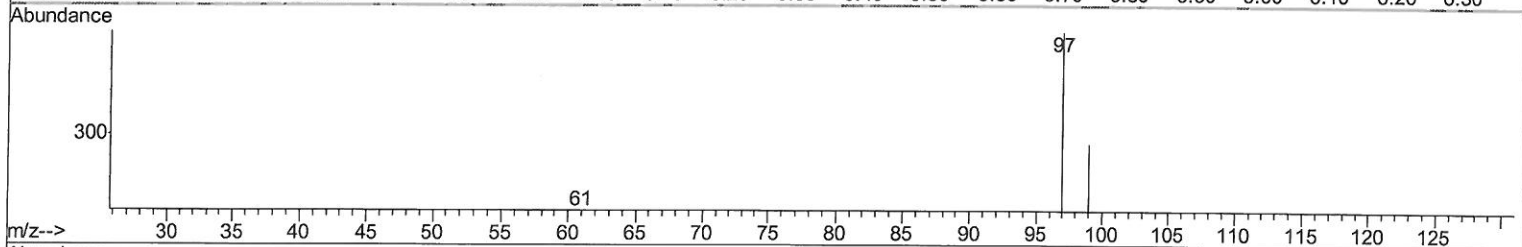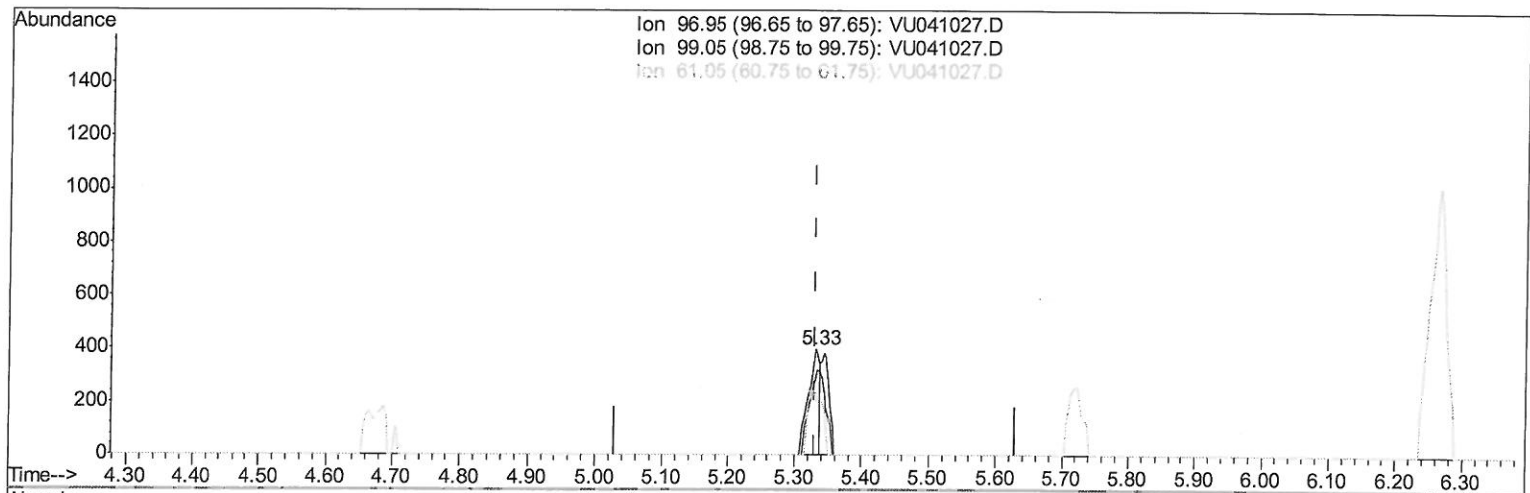

TIC: VU041027.D

(29) 1,1,1-Trichloroethane (T)

5.330min (-0.000) 0.07ug/L

response 460

Ion	Exp%	Act%
96.95	100	100
99.05	66.70	116.30#
61.05	52.00	79.57#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
 Data File : VU041027.D
 Acq On : 29 Oct 2020 20:36
 Operator : SY/MD
 Sample : L4558-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 C0BQ2

Manual Integrations
 APPROVED

MMDadoda
 11/2/2020 4:59:46 PM

Quant Time: Oct 30 09:17:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 30 08:06:28 2020
 Response via : Initial Calibration

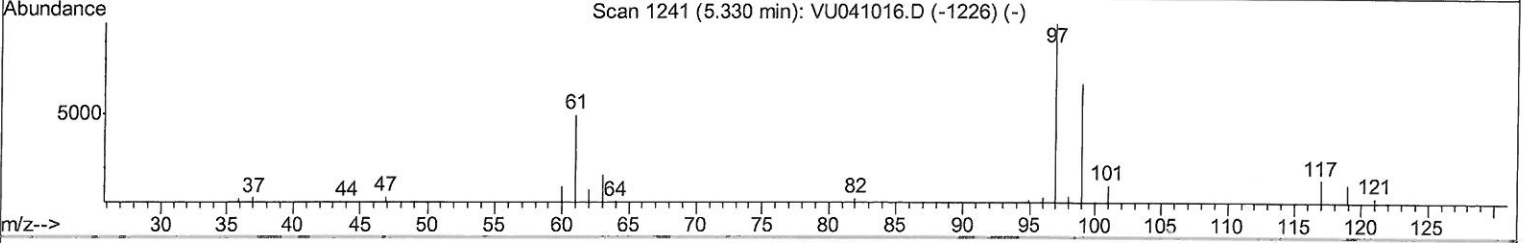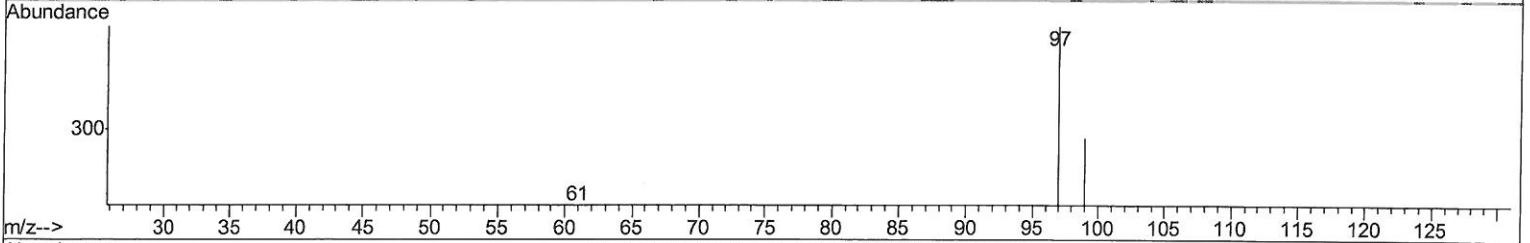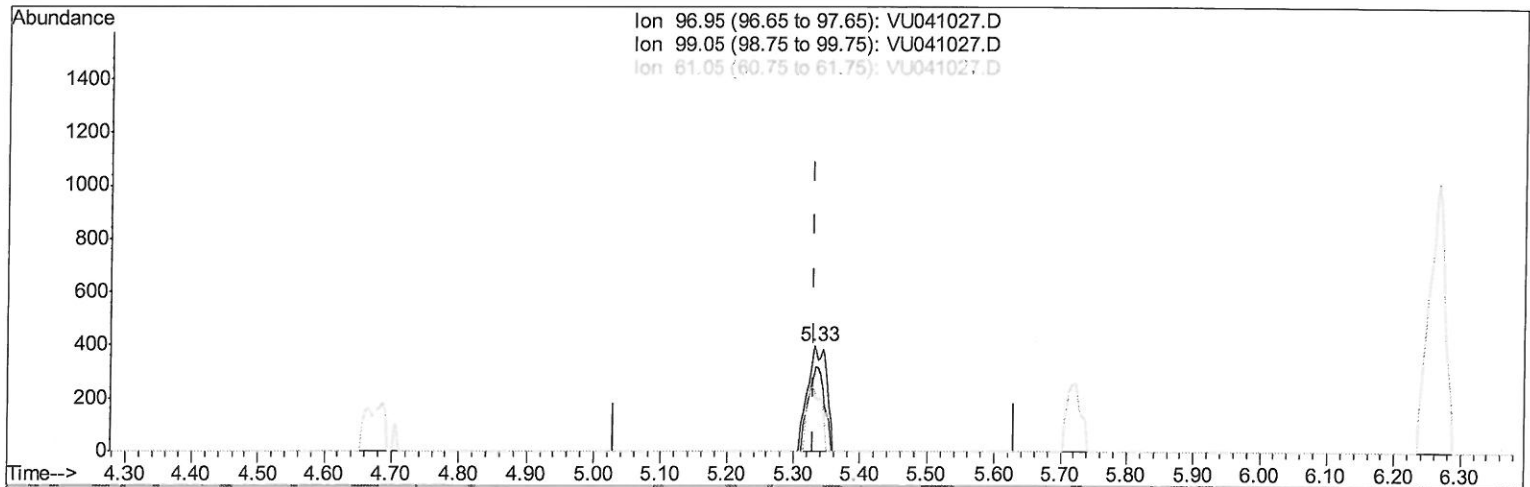

TIC: VU041027.D

(29) 1,1,1-Trichloroethane (T)

5.330min (-0.000) 0.12ug/L m

response 779

779
11/03/20

Ion	Exp%	Act%
96.95	100	100
99.05	66.70	68.68
61.05	52.00	46.98
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
 Data File : VU041027.D
 Acq On : 29 Oct 2020 20:36
 Operator : SY/MD
 Sample : L4558-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BQ2

Manual Integrations
 APPROVED

MMDadoda
 11/2/2020 4:59:46 PM

Quant Time: Oct 30 09:17:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 30 08:06:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	49828	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	52146	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	20838	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	15282	3.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.00%
7) Chloroethane-d5	1.92	69	12817	3.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.60%
11) 1,1-Dichloroethene-d2	2.58	63	24041	2.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.60%#
20) 2-Butanone-d5	4.66	46	80053	58.07	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.14%
24) Chloroform-d	5.08	84	33747	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.20%
26) 1,2-Dichloroethane-d4	5.72	65	22800	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.74	84	58617	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.00%
36) 1,2-Dichloropropane-d6	6.70	67	21702	4.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.60%
41) Toluene-d8	7.91	98	45895	3.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.60%
43) trans-1,3-Dichloropropene-	8.19	79	8075	4.10	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.00%
46) 2-Hexanone-d5	8.64	63	54527	51.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.90%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	20575	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	18859	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%

Target Compounds

					Ovalue
9) Trichlorofluoromethane	2.15	101	33781	5.311	ug/L 96
25) Chloroform	5.11	83	2398	0.334	ug/L 85
29) 1,1,1-Trichloroethane	5.33	97	779m	0.122	ug/L
31) Carbon tetrachloride	5.54	117	687	0.122	ug/L 88
34) Trichloroethene	6.55	95	4108	1.036	ug/L 95
47) Tetrachloroethene	8.56	164	28459	9.761	ug/L 99

MD
 11/03/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed