


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
Data File : VU041034.D
Acq On : 30 Oct 2020 10:57
Operator : SY/MD
Sample : L4558-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B82

Manual Integrations
APPROVED

MMDadoda
11/2/2020 4:59:54 PM

Quant Time: Oct 31 00:18:30 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 30 23:53:53 2020
Response via : Initial Calibration

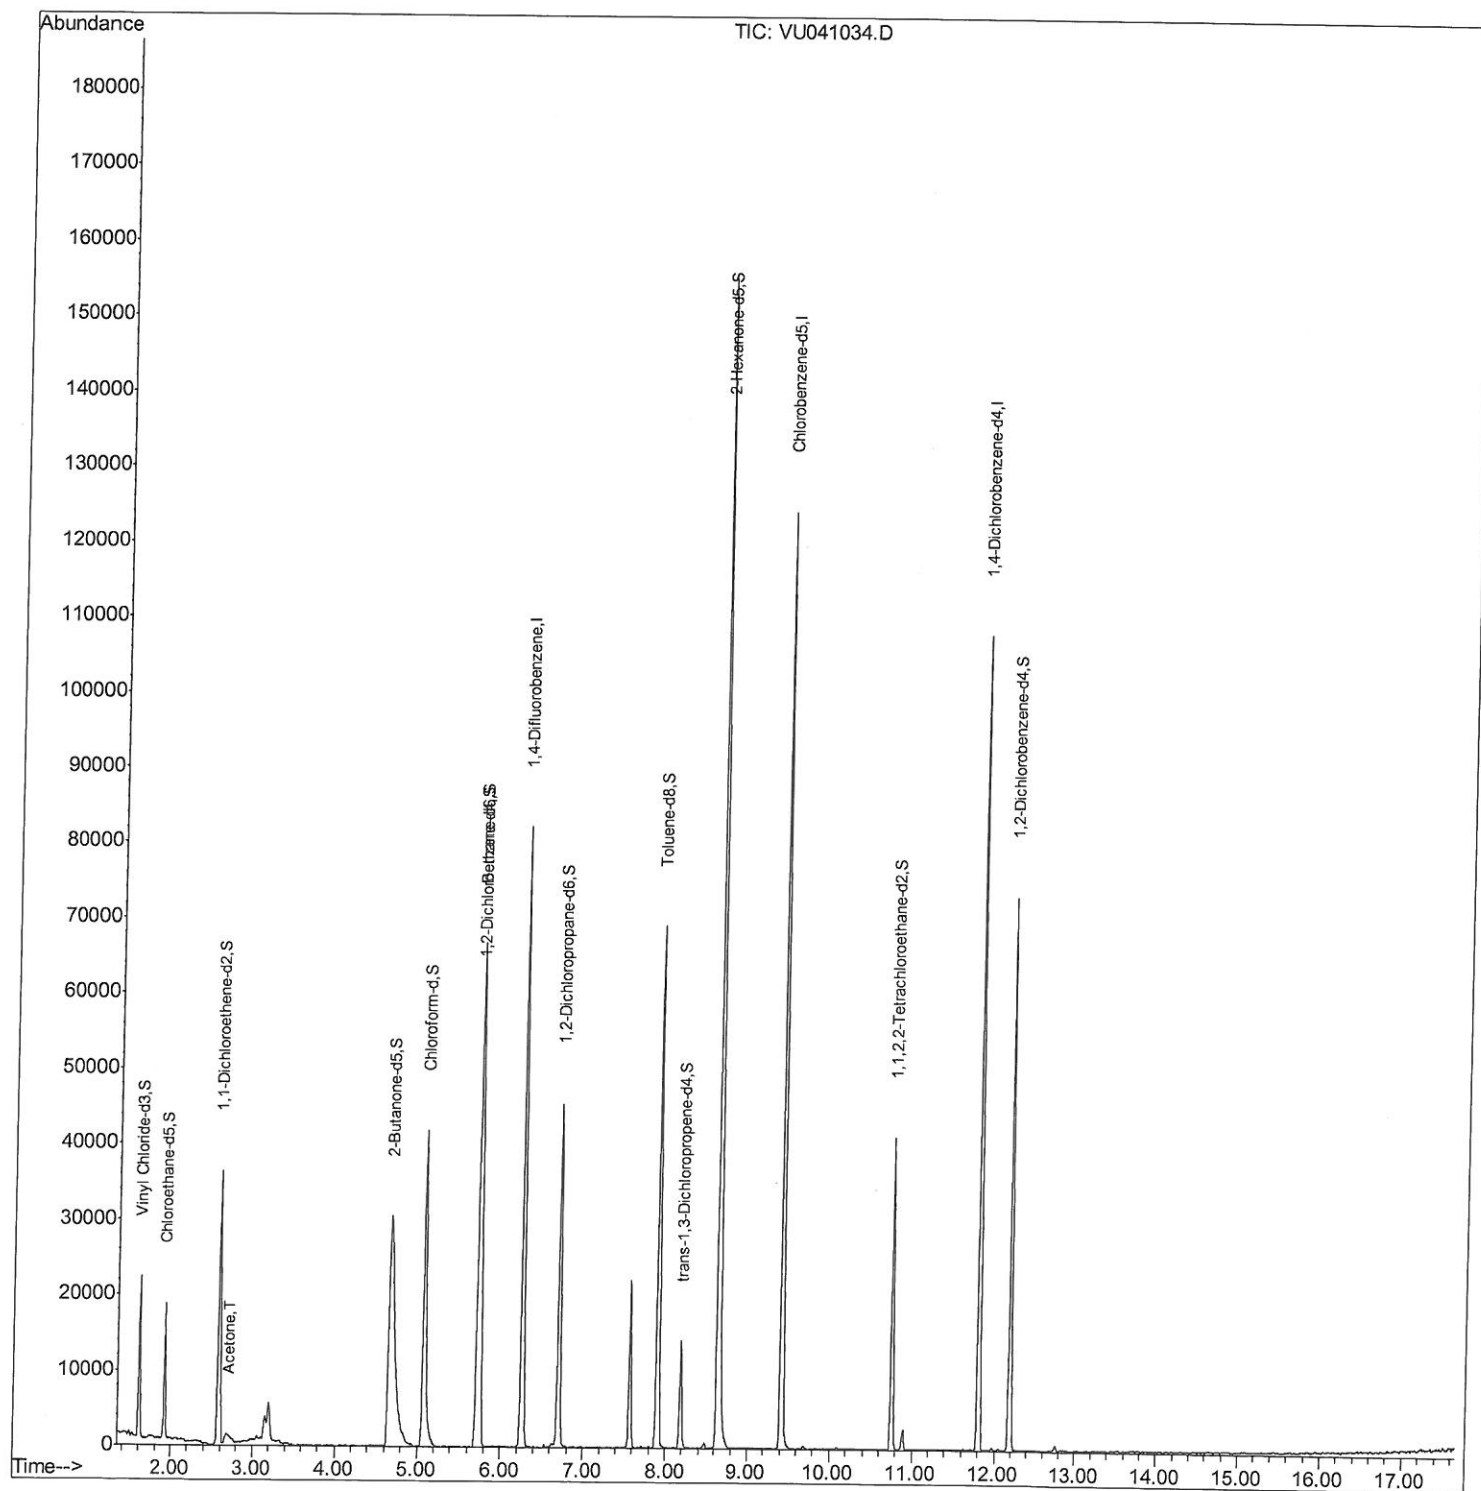

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
Data File : VU041034.D
Acq On : 30 Oct 2020 10:57
Operator : SY/MD
Sample : L4558-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B82

Manual Integrations
APPROVED

MMDadoda
11/2/2020 4:59:54 PM

Quant Time: Oct 31 00:01:23 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 30 23:53:53 2020
Response via : Initial Calibration

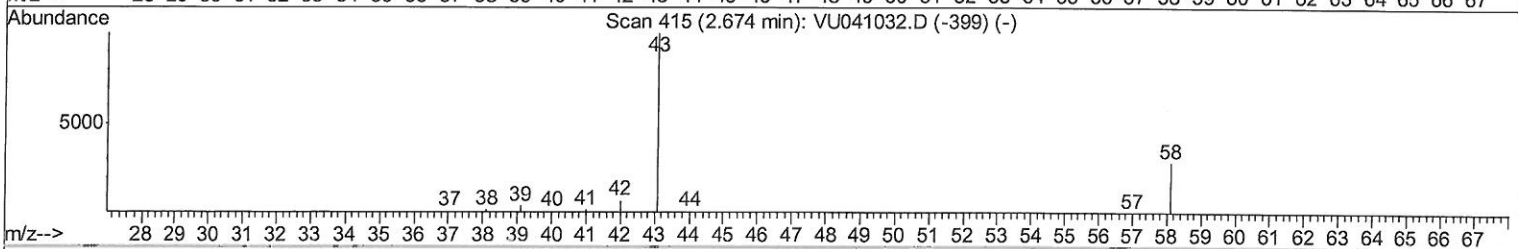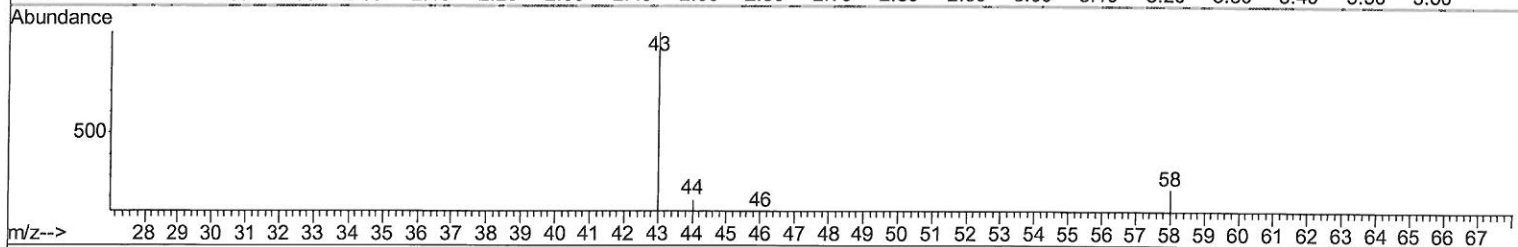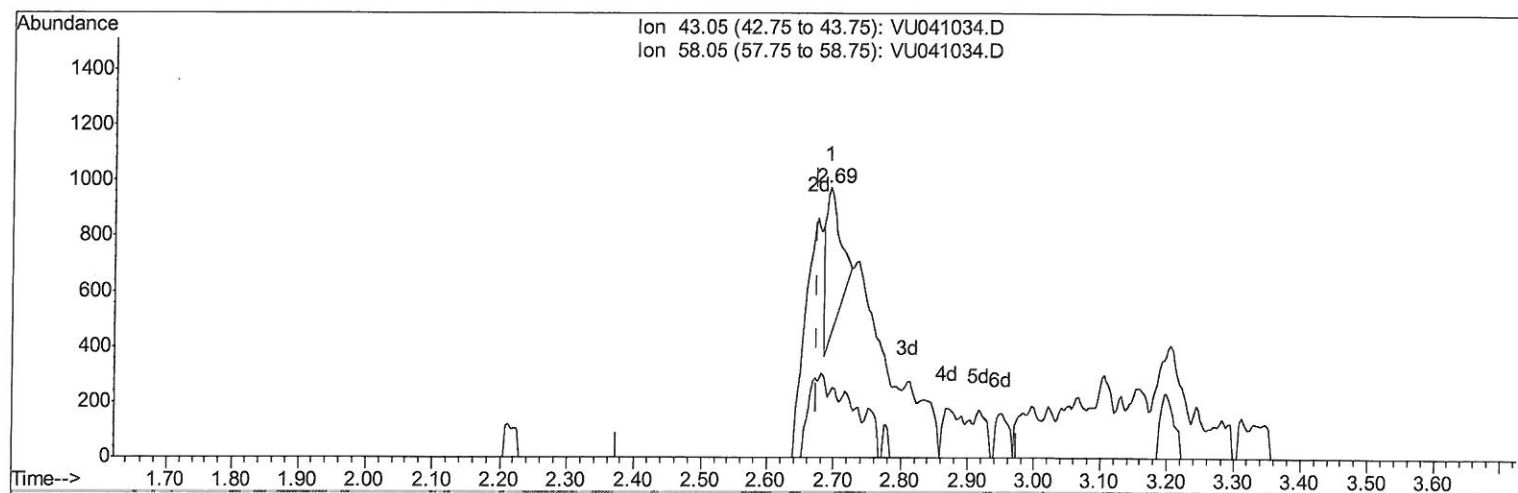

TIC: VU041034.D

(13) Acetone (T)

2.694min (+0.019) 0.62ug/L

response 724

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	17.40
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
 Data File : VU041034.D
 Acq On : 30 Oct 2020 10:57
 Operator : SY/MD
 Sample : L4558-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B82

Manual Integrations
 APPROVED

MMDadoda
 11/2/2020 4:59:54 PM

Quant Time: Oct 31 00:01:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 30 23:53:53 2020
 Response via : Initial Calibration

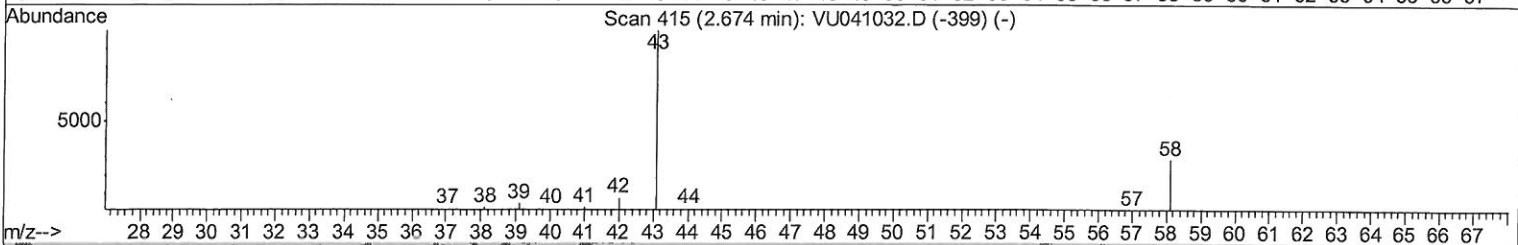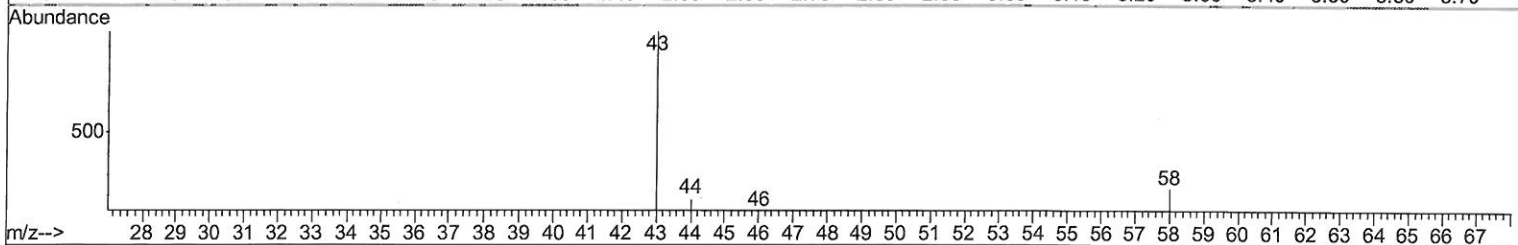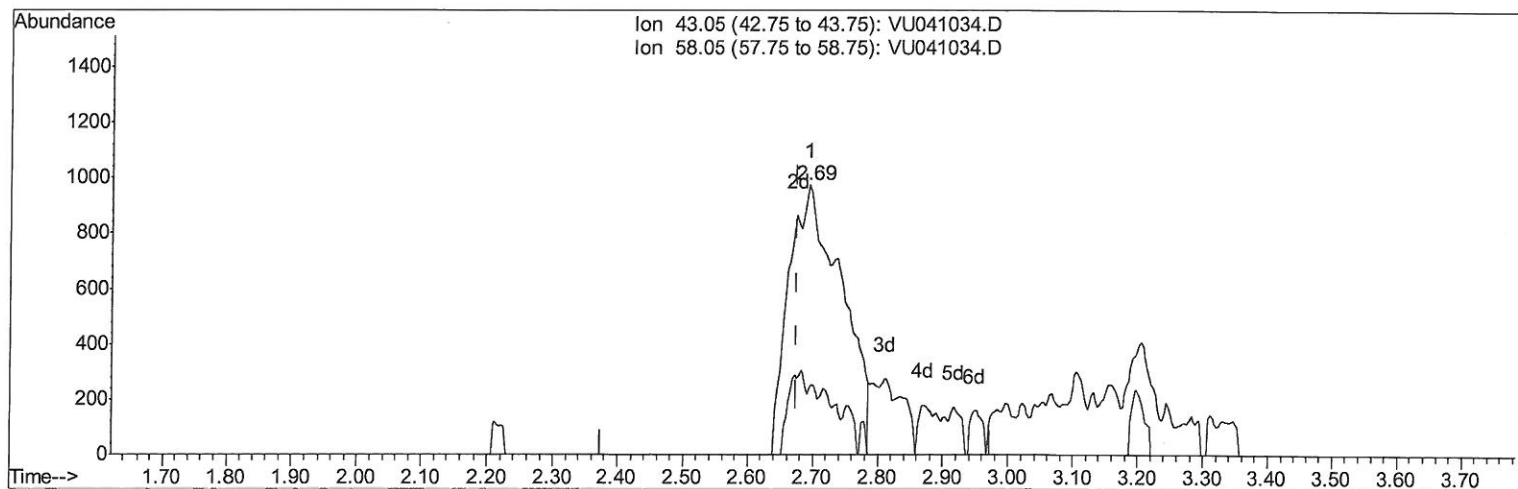

TIC: VU041034.D

(13) Acetone (T)

2.694min (+0.019) 4.65ug/L m

response 5432

MD
11/03/20

Ion	Exp%	Act%
43.05	100	100
58.05	12.70	2.32
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103020\
 Data File : VU041034.D
 Acq On : 30 Oct 2020 10:57
 Operator : SY/MD
 Sample : L4558-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 C0B82

Manual Integrations
 APPROVED

MMDadoda
 11/2/2020 4:59:54 PM

Quant Time: Oct 31 00:18:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 30 23:53:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	61718	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	61903	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	25604	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.61	65	14427	2.78	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	55.60%		
7) Chloroethane-d5	1.93	69	12564	3.15	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	63.00%#		
11) 1,1-Dichloroethene-d2	2.58	63	22422	2.20	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	44.00%#		
20) 2-Butanone-d5	4.66	46	79897	46.79	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	93.58%		
24) Chloroform-d	5.08	84	32782	3.58	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	71.60%		
26) 1,2-Dichloroethane-d4	5.72	65	22238	3.91	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	78.20%		
32) Benzene-d6	5.74	84	55821	3.37	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	67.40%#		
36) 1,2-Dichloropropane-d6	6.70	67	20589	3.82	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	76.40%		
41) Toluene-d8	7.90	98	43692	2.91	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	58.20%#		
43) trans-1,3-Dichloropropene-	8.18	79	8214	3.51	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	70.20%		
46) 2-Hexanone-d5	8.64	63	52897	42.05	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	84.10%		
57) 1,1,2,2-Tetrachloroethane-	10.75	84	20094	4.01	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	80.20%		
64) 1,2-Dichlorobenzene-d4	12.19	152	17991	4.00	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	80.00%		

Target Compounds				Ovalue
13) Acetone	2.69	43	5432m	4.653 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 MB
 11/03/20