


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU103020\
 Data File : VU041015.D
 Acq On : 29 Oct 2020 13:48
 Operator : SY/MD
 Sample : BFB01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Oct 30 08:06:28 2020

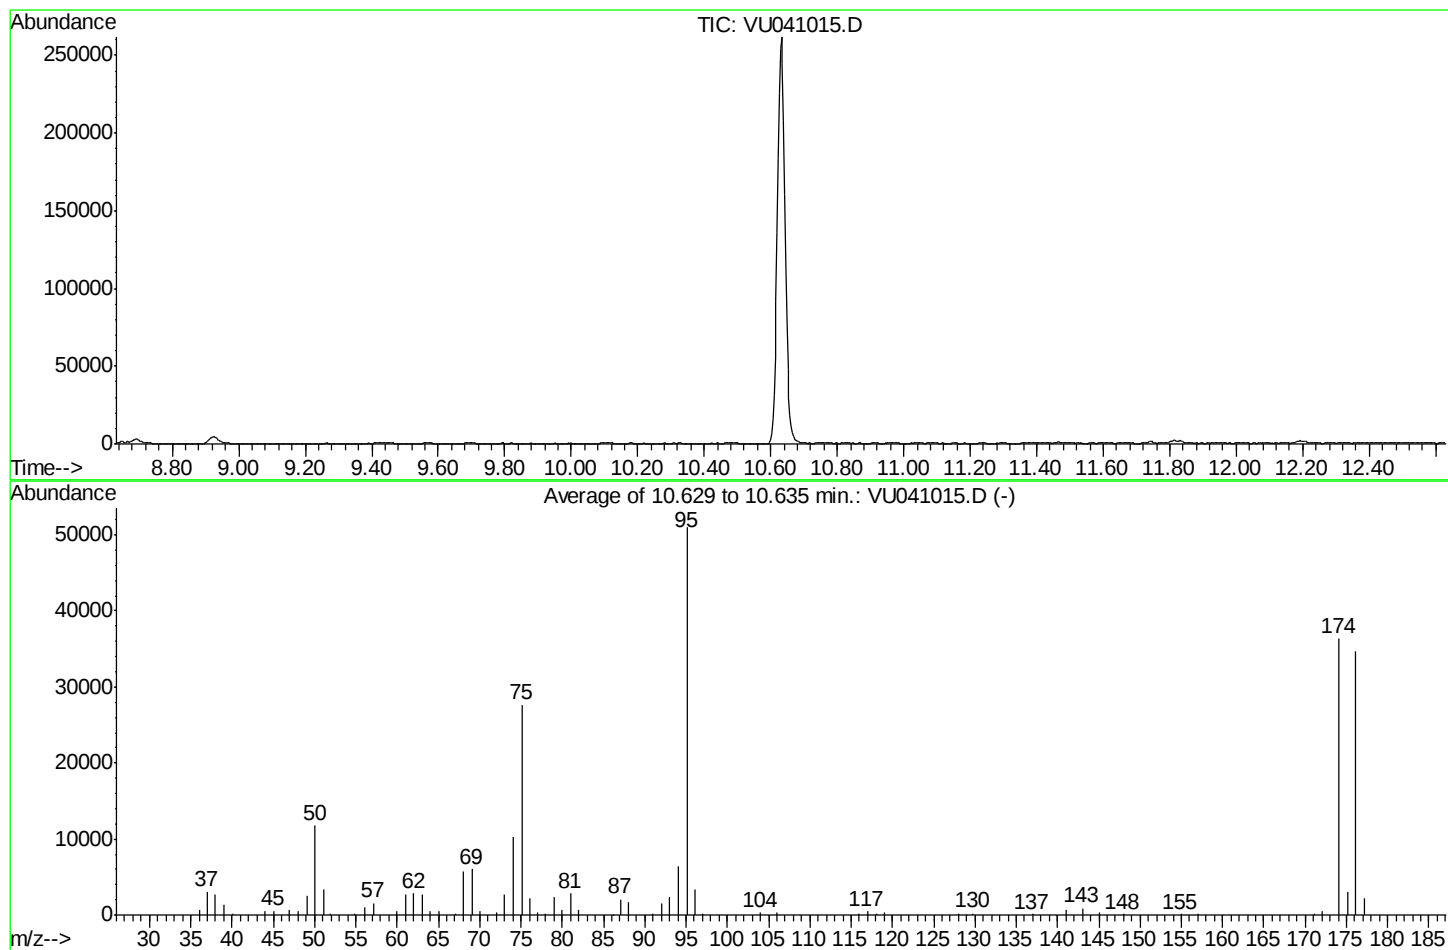

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	11718	PASS
75	95	30	80	54.2	27653	PASS
95	95	100	100	100.0	51000	PASS
96	95	5	9	6.5	3301	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.2	36296	PASS
175	174	5	9	8.2	2968	PASS
176	174	95	101	95.6	34709	PASS
177	176	5	9	6.2	2137	PASS

m/z	Abundance
36.00	643.0
37.00	3332.0
38.00	2801.0
39.00	1244.0
40.10	187.0
44.00	762.0
45.00	540.0
47.00	614.0
48.00	373.0
49.10	2579.0
50.10	12046.0
51.10	3520.0
52.00	151.0
54.90	167.0
56.10	1092.0
57.10	1512.0
60.00	531.0
61.10	2672.0
62.00	2926.0
63.00	2645.0
64.10	516.0
65.10	555.0
68.10	5686.0
69.10	6006.0
70.10	432.0
72.00	404.0
73.00	2612.0
74.10	10236.0
75.10	28176.0
76.10	2308.0
77.00	412.0
78.00	201.0
79.00	2410.0
80.00	658.0
81.00	2844.0
81.90	657.0
86.10	135.0
87.00	2051.0
88.00	1720.0
91.00	285.0
92.00	1428.0
93.00	2389.0
94.10	6498.0
95.10	51568.0
96.10	3490.0
97.00	106.0
104.00	291.0
106.00	289.0
116.00	226.0
117.00	440.0
118.00	208.0
119.00	355.0
128.00	209.0
129.80	251.0
137.00	136.0
141.00	640.0
143.00	833.0
145.10	319.0
148.00	157.0
155.00	150.0
157.00	120.0
171.10	198.0
172.00	446.0
174.10	35752.0
175.10	2981.0
176.10	34152.0
177.10	2111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	677.0
37.00	3143.0
38.00	2849.0
39.00	1329.0
40.10	157.0
44.00	779.0
45.00	564.0
47.00	616.0
48.10	454.0
49.00	2721.0
50.10	12278.0
51.10	3558.0
52.00	166.0
54.90	164.0
56.00	1049.0
57.10	1577.0
60.00	569.0
61.10	2741.0
62.00	2963.0
63.00	2783.0
64.10	473.0
65.00	518.0
67.20	197.0
68.10	5980.0
69.00	6307.0
70.00	477.0
72.00	374.0
73.00	2724.0
74.10	10664.0
75.10	28648.0
76.10	2249.0
77.00	413.0
77.90	195.0
79.00	2448.0
80.00	682.0
81.00	2945.0
81.90	711.0
87.10	2090.0
88.00	1728.0
91.00	241.0
92.00	1623.0
93.00	2484.0
94.10	6543.0
95.10	52456.0
96.10	3436.0
97.00	133.0
104.00	331.0
106.00	297.0
115.90	217.0
117.00	511.0
118.10	214.0
119.00	414.0
128.00	192.0
129.80	202.0
137.00	136.0
141.00	764.0
143.00	904.0
145.00	339.0
148.00	165.0
155.00	143.0
157.00	134.0
171.00	221.0
172.10	459.0
174.10	37320.0
175.10	3076.0
176.10	35712.0
177.10	2175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	675.0
37.00	2791.0
38.00	2651.0
39.00	1304.0
40.00	130.0
44.00	726.0
45.00	526.0
47.00	591.0
48.10	466.0
49.00	2451.0
50.10	10830.0
51.10	3136.0
51.90	164.0
54.90	154.0
56.00	931.0
57.10	1583.0
60.00	518.0
61.10	2677.0
62.00	2646.0
63.00	2505.0
64.00	405.0
65.00	497.0
67.00	208.0
68.00	5564.0
69.10	5691.0
70.10	498.0
72.00	257.0
73.10	2589.0
74.10	10076.0
75.10	26136.0
76.00	2065.0
77.00	370.0
77.90	177.0
79.00	2383.0
80.00	619.0
81.00	2601.0
81.90	692.0
87.10	1954.0
88.00	1487.0
91.00	160.0
92.00	1623.0
93.10	2335.0
94.10	6090.0
95.10	48976.0
96.10	2977.0
97.10	137.0
104.00	307.0
106.00	323.0
115.90	230.0
117.00	506.0
118.00	180.0
119.00	426.0
128.00	155.0
129.00	101.0
129.90	126.0
136.90	109.0
141.00	736.0
143.10	883.0
145.00	325.0
148.00	143.0
155.00	131.0
157.10	120.0
171.00	229.0
172.10	494.0
174.10	35816.0
175.10	2847.0
176.10	34264.0
177.10	2125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
44.00	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01