


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU103020\
Data File : VU041031.D
Acq On : 30 Oct 2020 09:00
Operator : SY/MD
Sample : BFB02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB02

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Oct 30 23:53:53 2020

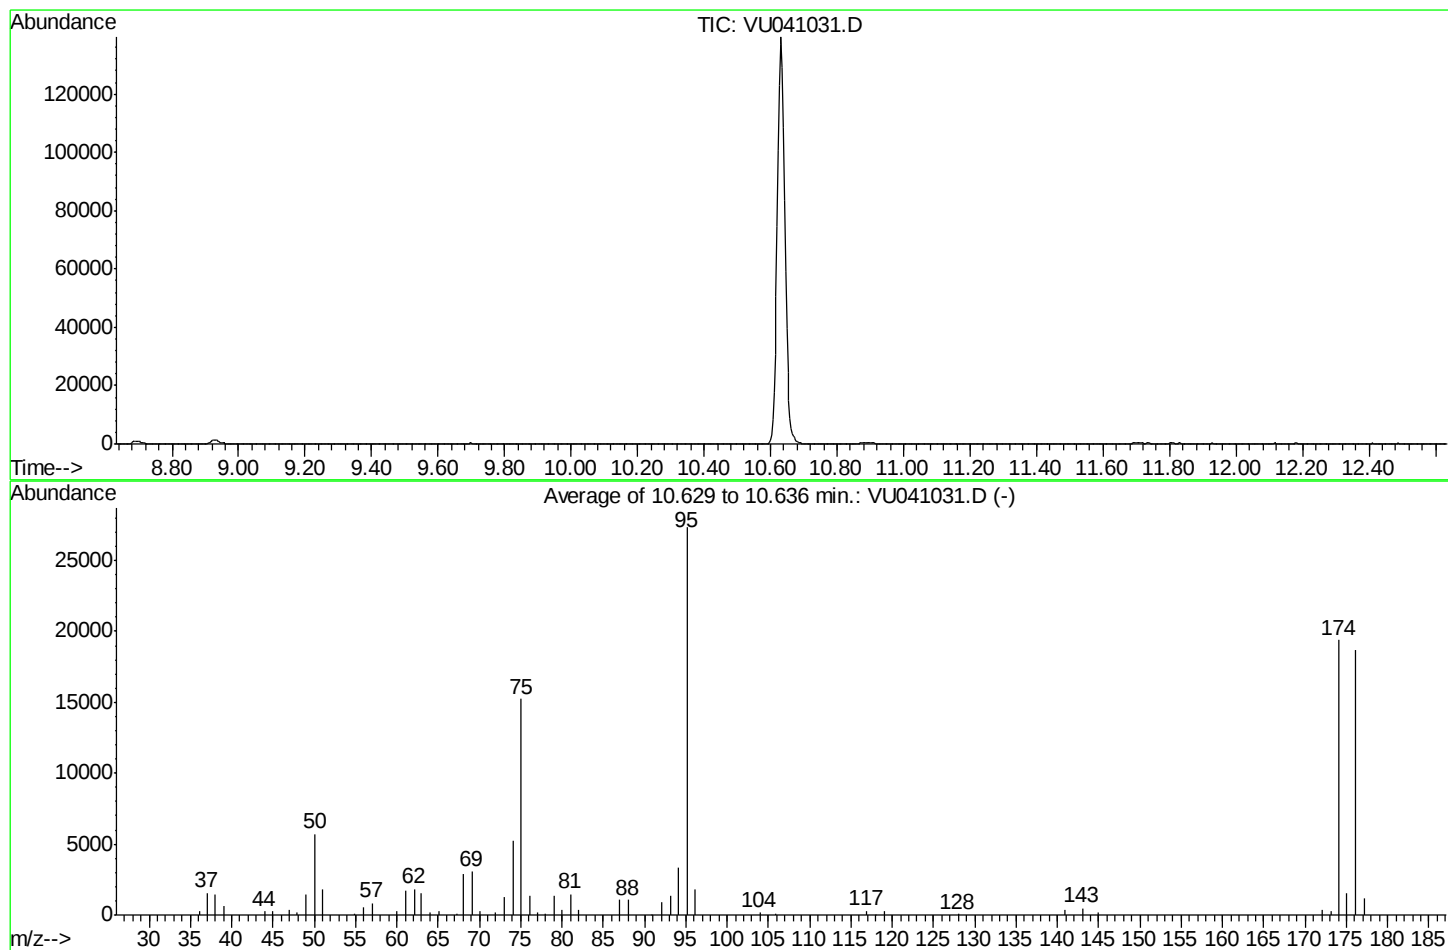

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	5708	PASS
75	95	30	80	55.8	15248	PASS
95	95	100	100	100.0	27338	PASS
96	95	5	9	6.8	1849	PASS
173	174	0.00	2	1.6	309	PASS
174	95	50	120	70.9	19378	PASS
175	174	5	9	7.8	1503	PASS
176	174	95	101	96.7	18730	PASS
177	176	5	9	6.5	1214	PASS

m/z	Abundance
36.00	293.0
37.00	1550.0
38.00	1543.0
39.10	648.0
44.00	367.0
45.00	244.0
47.00	347.0
47.90	188.0
49.00	1520.0
50.10	5855.0
51.00	1841.0
54.90	107.0
56.00	591.0
57.00	912.0
60.00	264.0
61.00	1780.0
62.10	1805.0
63.00	1560.0
64.00	236.0
65.10	320.0
67.20	135.0
68.10	3068.0
69.10	3051.0
70.00	266.0
72.10	153.0
73.10	1302.0
74.10	5304.0
75.10	15567.0
76.10	1294.0
77.00	161.0
79.00	1435.0
80.00	407.0
81.00	1504.0
81.90	357.0
87.00	1087.0
88.00	1150.0
90.90	127.0
92.00	864.0
93.10	1396.0
94.10	3411.0
95.10	27984.0
96.10	1978.0
103.90	138.0
105.90	147.0
116.90	281.0
119.00	281.0
140.90	315.0
143.00	494.0
145.00	189.0
172.00	358.0
173.10	463.0
174.10	19216.0
175.10	1459.0
176.10	18568.0
177.10	1223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.10	265.0
37.00	1609.0
38.00	1474.0
39.00	650.0
44.00	374.0
45.00	249.0
47.00	383.0
48.00	174.0
49.00	1537.0
50.10	5909.0
51.10	1843.0
55.00	127.0
56.00	568.0
57.00	890.0
60.00	253.0
61.00	1777.0
62.10	1916.0
63.00	1540.0
64.00	218.0
65.10	318.0
67.20	124.0
68.10	3007.0
69.10	3145.0
70.00	263.0
72.00	140.0
73.00	1256.0
74.10	5384.0
75.10	15685.0
76.10	1346.0
77.00	175.0
77.90	130.0
79.00	1417.0
80.00	431.0
81.00	1531.0
82.00	355.0
87.00	1114.0
88.00	1110.0
92.00	928.0
93.10	1439.0
94.10	3468.0
95.10	28208.0
96.10	1904.0
104.00	150.0
106.00	126.0
117.00	316.0
119.00	273.0
128.00	105.0
140.90	313.0
143.00	517.0
144.90	176.0
172.00	426.0
173.10	466.0
174.10	19984.0
175.10	1552.0
176.10	19312.0
177.10	1219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.10	238.0
37.00	1550.0
38.00	1348.0
39.00	614.0
44.00	379.0
45.00	218.0
47.00	352.0
48.00	160.0
49.00	1390.0
50.10	5361.0
51.10	1689.0
54.90	123.0
56.00	486.0
57.00	767.0
60.00	252.0
61.00	1588.0
62.10	1741.0
63.00	1423.0
64.10	212.0
65.10	274.0
68.00	2627.0
69.10	2937.0
70.00	238.0
71.90	139.0
73.00	1247.0
74.10	4945.0
75.10	14493.0
76.10	1310.0
77.00	175.0
78.00	144.0
79.00	1220.0
80.00	388.0
81.00	1413.0
82.00	324.0
87.00	977.0
88.10	968.0
92.00	907.0
93.10	1291.0
94.10	3144.0
95.10	25824.0
96.10	1667.0
104.00	142.0
106.00	102.0
117.00	308.0
118.00	109.0
119.10	214.0
128.00	122.0
141.00	333.0
143.00	481.0
144.90	139.0
172.00	437.0
174.10	18936.0
175.00	1500.0
176.10	18312.0
177.10	1201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
44.00	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02