

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
 Data File : VU055998.D
 Acq On : 30 Oct 2023 15:36
 Operator : MD/SY
 Sample : 05113-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B71

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU055998.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	109	rBV	129628	153345	11.55%	1.366%
2	1.914	185	194	215	rVB	112304	153252	11.54%	1.365%
3	2.566	385	397	411	rBV	223614	367469	27.68%	3.272%
4	2.792	453	467	477	rBV2	10201	21294	1.60%	0.190%
5	3.193	574	592	617	rBV4	23560	92356	6.96%	0.822%
6	4.627	1019	1038	1084	rBV	158525	498331	37.54%	4.438%
7	5.058	1156	1172	1196	rBV	222388	502156	37.82%	4.472%
8	5.724	1358	1379	1404	rBV2	437318	1144429	86.20%	10.191%
9	6.248	1527	1542	1572	rBV	409053	814794	61.37%	7.256%
10	6.688	1664	1679	1702	rBV	266874	537342	40.48%	4.785%
11	7.563	1936	1951	1974	rBV	121856	230737	17.38%	2.055%
12	7.897	2036	2055	2075	rBV	506531	929741	70.03%	8.279%
13	8.177	2132	2142	2159	rBV	73428	132564	9.99%	1.180%
14	8.550	2244	2258	2273	rBV	781295	1327584	100.00%	11.822%
15	8.634	2273	2284	2325	rVB3	511855	1158447	87.26%	10.316%
16	9.415	2514	2527	2555	rBV	584919	1036775	78.09%	9.232%
17	10.753	2929	2943	2961	rBV	199749	329048	24.79%	2.930%
18	10.888	2975	2985	2996	rBV2	11828	20540	1.55%	0.183%
19	11.810	3259	3272	3293	rBV	577317	961307	72.41%	8.560%
20	12.190	3371	3390	3407	rBV	481833	818278	61.64%	7.287%




Sum of corrected areas: 11229789

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU055998.D
Acq On : 30 Oct 2023 15:36
Operator : MD/SY
Sample : 05113-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

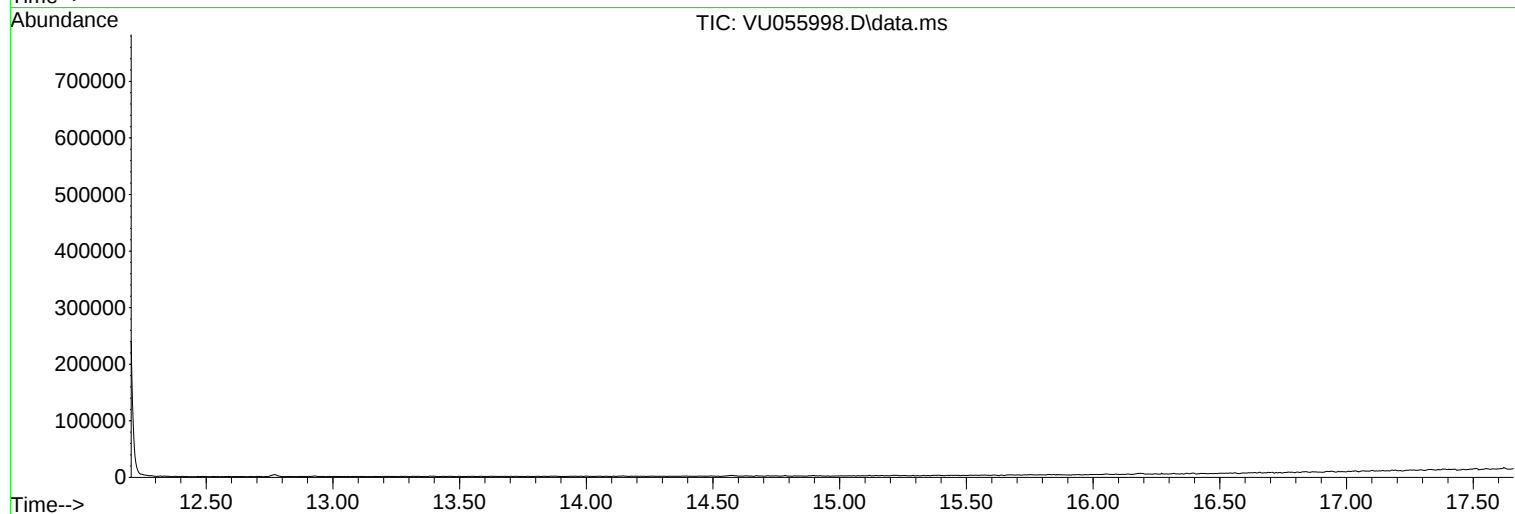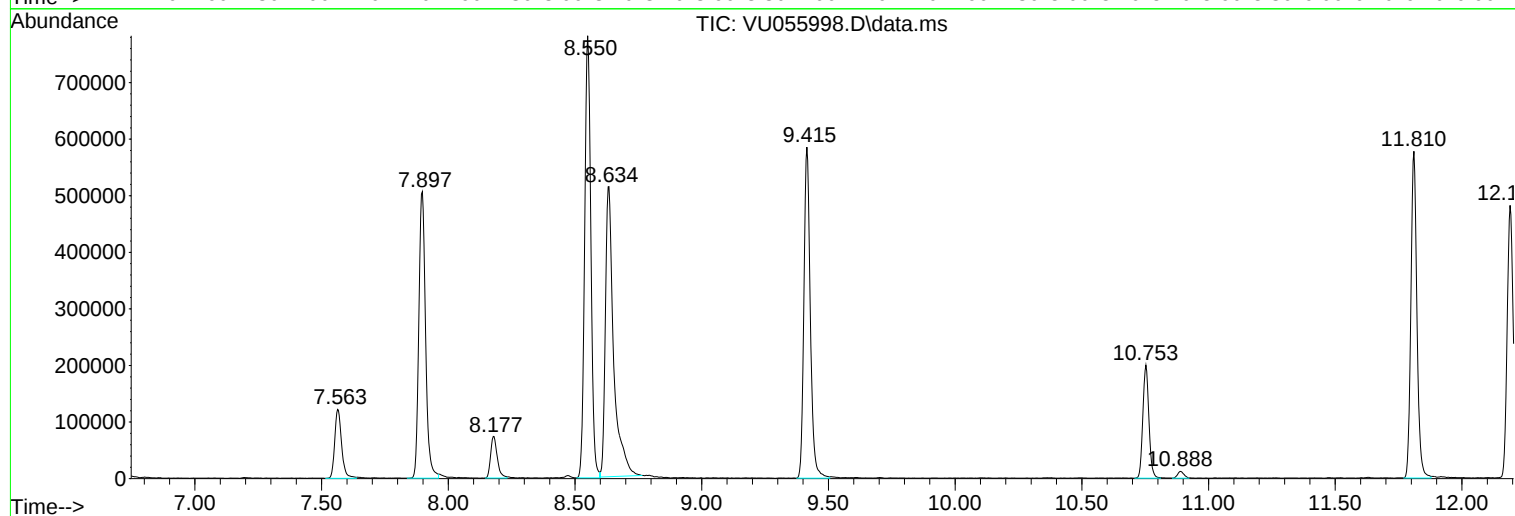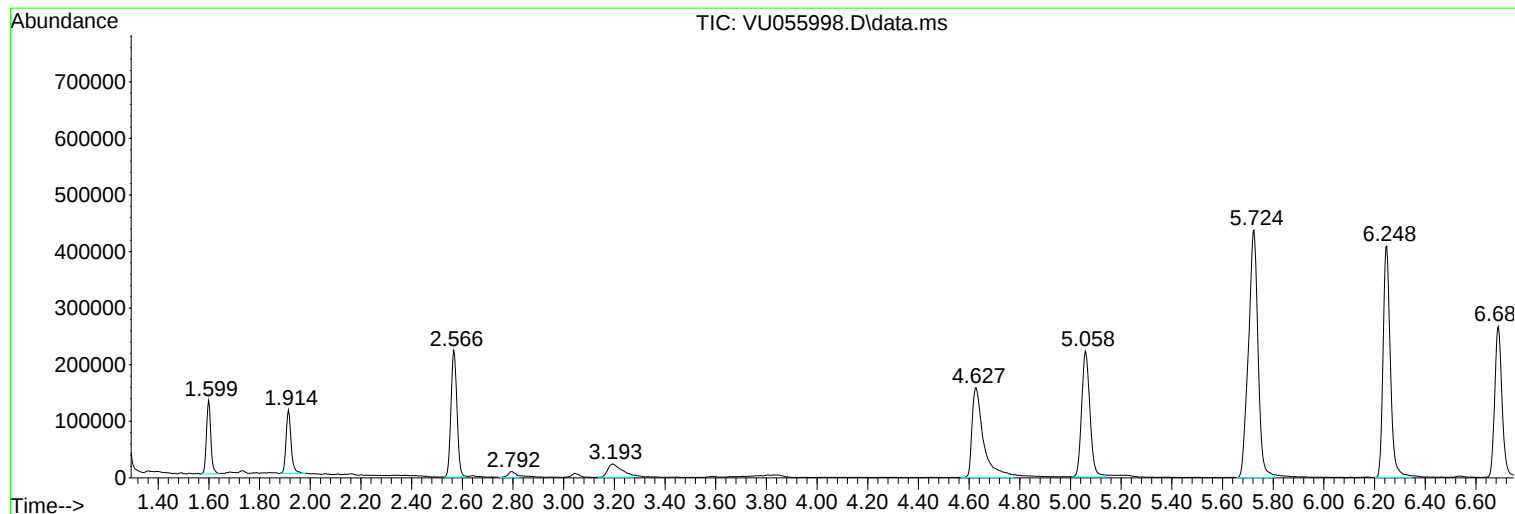

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU055998.D
Acq On : 30 Oct 2023 15:36
Operator : MD/SY
Sample : 05113-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B71










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.193	0.57 ug/L	92356	1,4-Difluorobenzene	6.248

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	HEX-5-EN-3-OL			100	C6H12O	000688-99-3	40
2	2-Propanol, 2-methyl-			74	C4H10O	000075-65-0	40
3	3-Pentanol			88	C5H12O	000584-02-1	40
4	L-Threonine, O-methyl-, methyl e...			147	C6H13NO3	1000452-62-7	40
5	3-Pentanol			88	C5H12O	000584-02-1	33

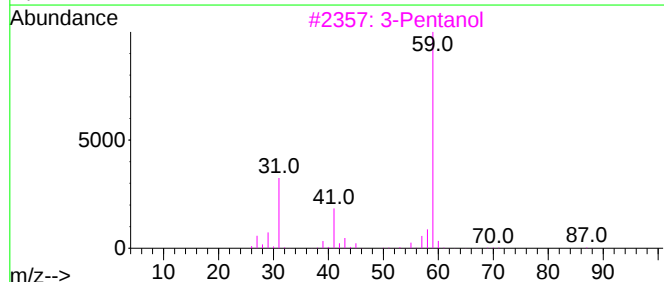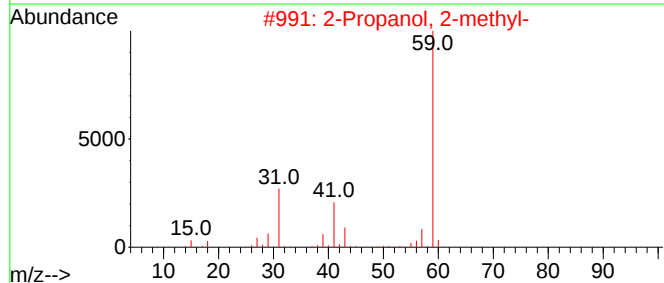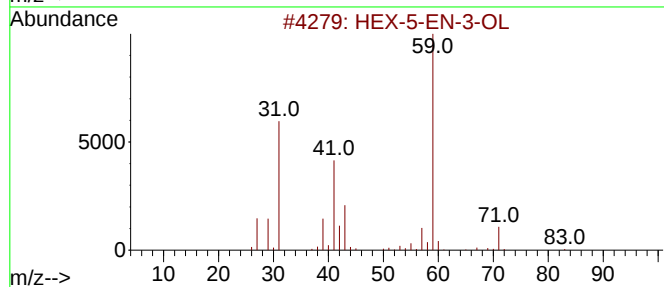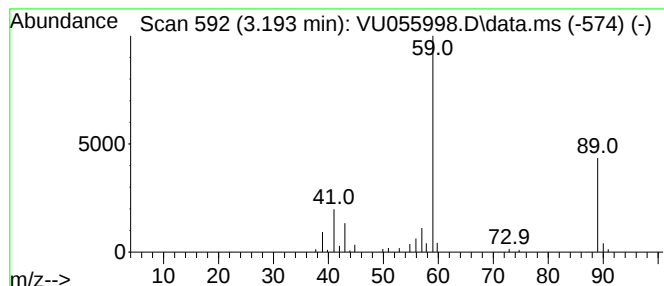

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU055998.D
Acq On : 30 Oct 2023 15:36
Operator : MD/SY
Sample : 05113-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.193	0.6	ug/L	92356	1	6.248	814794	5.0