

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
 Data File : VU056003.D
 Acq On : 30 Oct 2023 17:36
 Operator : MD/SY
 Sample : 05113-11 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	107	rBV	128972	145030	8.55%	1.289%
2	1.914	186	194	211	rVB	113573	157377	9.28%	1.399%
3	2.566	384	397	414	rVB	217811	359470	21.19%	3.196%
4	3.046	534	546	565	rVB3	8376	18274	1.08%	0.162%
5	4.627	1023	1038	1080	rBV	143770	448739	26.46%	3.990%
6	5.058	1156	1172	1208	rVB	223271	510522	30.10%	4.539%
7	5.724	1356	1379	1416	rBV3	432463	1141554	67.30%	10.149%
8	6.248	1529	1542	1571	rBV	394160	782203	46.12%	6.954%
9	6.688	1665	1679	1704	rBV	268526	538734	31.76%	4.790%
10	7.563	1939	1951	1973	rBV	123597	230880	13.61%	2.053%
11	7.897	2042	2055	2076	rBV	507612	919618	54.22%	8.176%
12	8.180	2131	2143	2159	rBV2	72012	129268	7.62%	1.149%
13	8.550	2244	2258	2273	rBV	981216	1696128	100.00%	15.080%
14	8.634	2273	2284	2325	rVB3	500588	1145117	67.51%	10.181%
15	9.415	2514	2527	2560	rBV	558582	981293	57.85%	8.725%
16	10.753	2930	2943	2963	rBV	194960	326373	19.24%	2.902%
17	10.891	2975	2986	2999	rVB2	12754	21118	1.25%	0.188%
18	11.810	3259	3272	3294	rBV	533815	899558	53.04%	7.998%
19	12.190	3377	3390	3416	rBV	459139	796270	46.95%	7.080%




Sum of corrected areas: 11247526

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU056003.D
Acq On : 30 Oct 2023 17:36
Operator : MD/SY
Sample : 05113-11 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

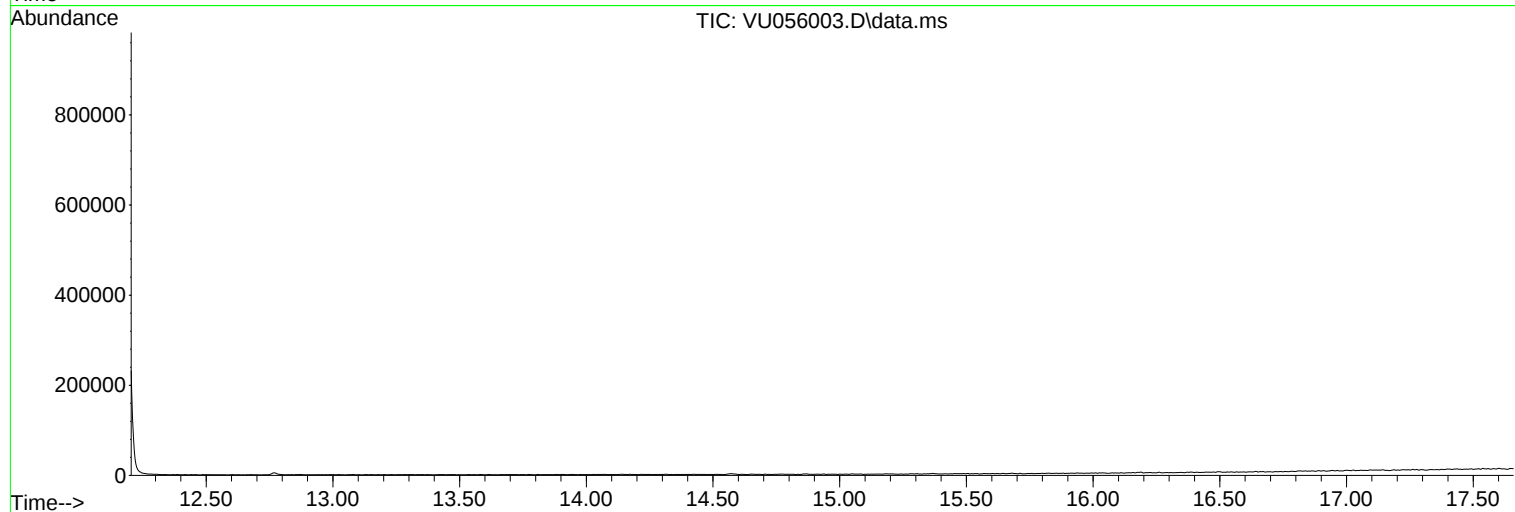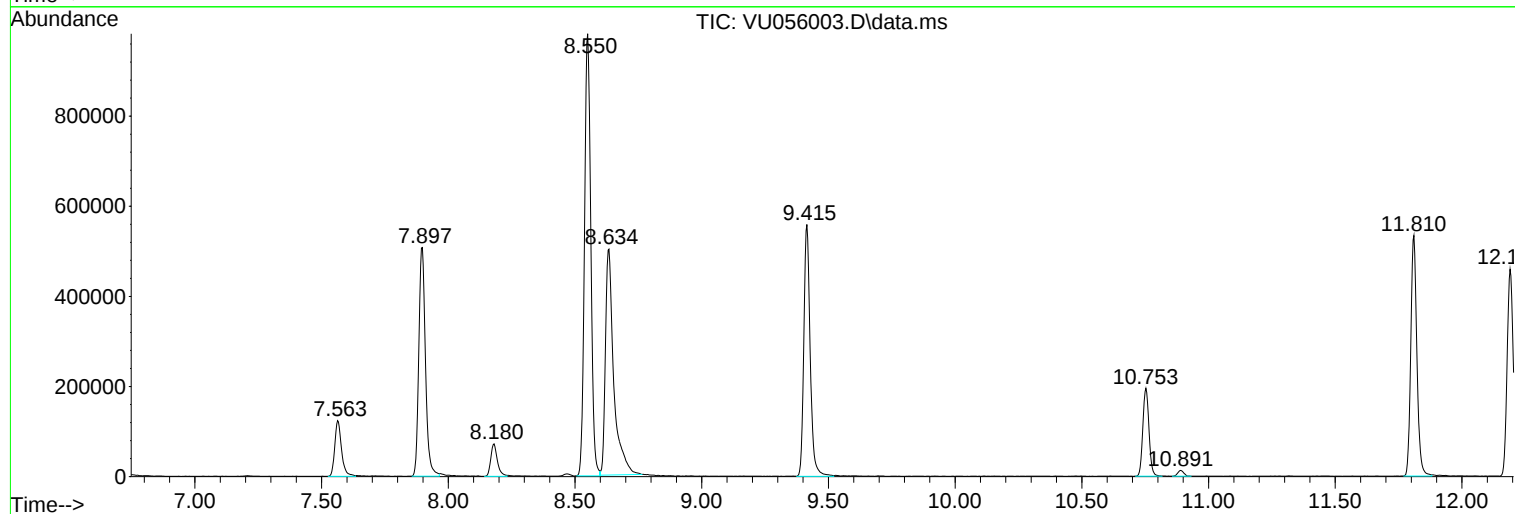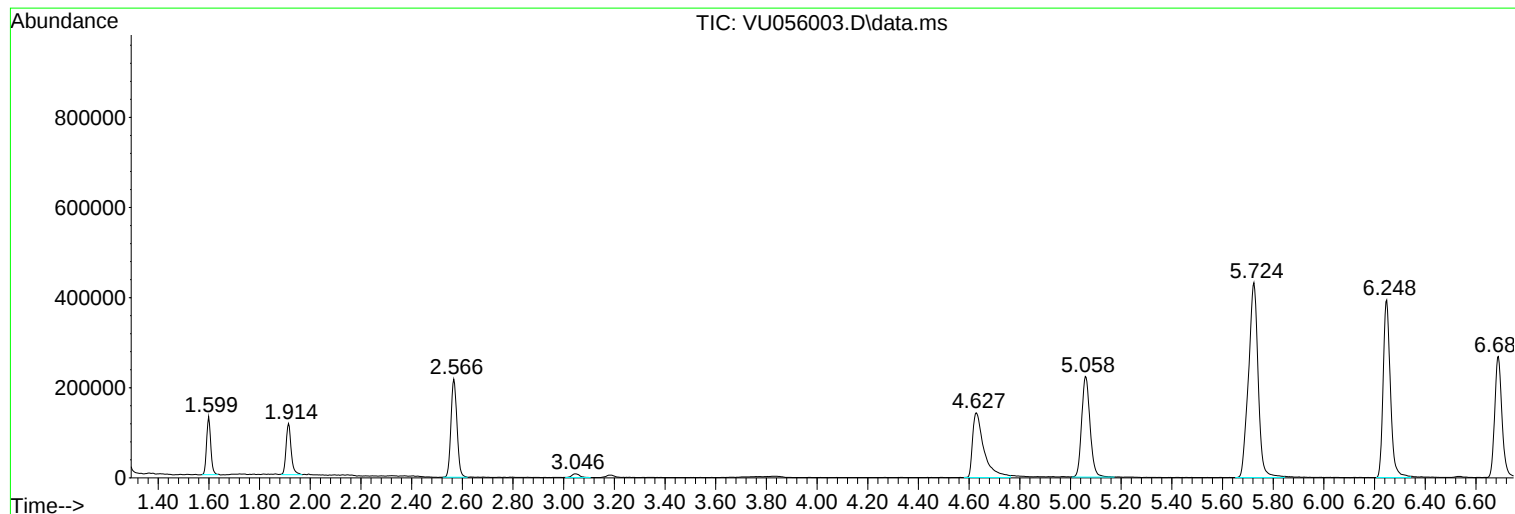

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU056003.D
Acq On : 30 Oct 2023 17:36
Operator : MD/SY
Sample : 05113-11 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU056003.D
Acq On : 30 Oct 2023 17:36
Operator : MD/SY
Sample : 05113-11 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc