

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
 Data File : VU056004.D
 Acq On : 30 Oct 2023 18:00
 Operator : MD/SY
 Sample : 05114-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B73

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056004.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	110	rVB	122002	141873	7.60%	1.281%
2	1.914	185	194	209	rBV	107049	145440	7.79%	1.314%
3	2.567	383	397	411	rBV	212550	349050	18.70%	3.153%
4	3.197	574	593	612	rBV3	20217	80483	4.31%	0.727%
5	4.628	1022	1038	1095	rBV2	146990	494870	26.51%	4.470%
6	5.081	1155	1179	1212	rBV2	679447	1867012	100.00%	16.863%
7	5.724	1358	1379	1405	rBV2	426578	1110016	59.45%	10.026%
8	6.245	1527	1541	1577	rBV	368003	737726	39.51%	6.663%
9	6.685	1663	1678	1712	rBV	257827	521350	27.92%	4.709%
10	7.103	1794	1808	1827	rBV	151857	287077	15.38%	2.593%
11	7.563	1936	1951	1983	rBV2	119114	221524	11.87%	2.001%
12	7.894	2040	2054	2074	rBV	479316	876333	46.94%	7.915%
13	8.181	2132	2143	2166	rBV2	68139	127046	6.80%	1.147%
14	8.634	2272	2284	2325	rBV2	489282	1128843	60.46%	10.196%
15	8.804	2327	2337	2353	rVB	33322	63017	3.38%	0.569%
16	9.415	2513	2527	2562	rBV	521651	939431	50.32%	8.485%
17	10.753	2928	2943	2961	rBV	189524	318848	17.08%	2.880%
18	10.888	2976	2985	2998	rVB3	13675	23481	1.26%	0.212%
19	11.811	3259	3272	3293	rBV	516628	861578	46.15%	7.782%
20	12.190	3377	3390	3421	rBV	450728	776725	41.60%	7.015%




Sum of corrected areas: 11071723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU056004.D
Acq On : 30 Oct 2023 18:00
Operator : MD/SY
Sample : 05114-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

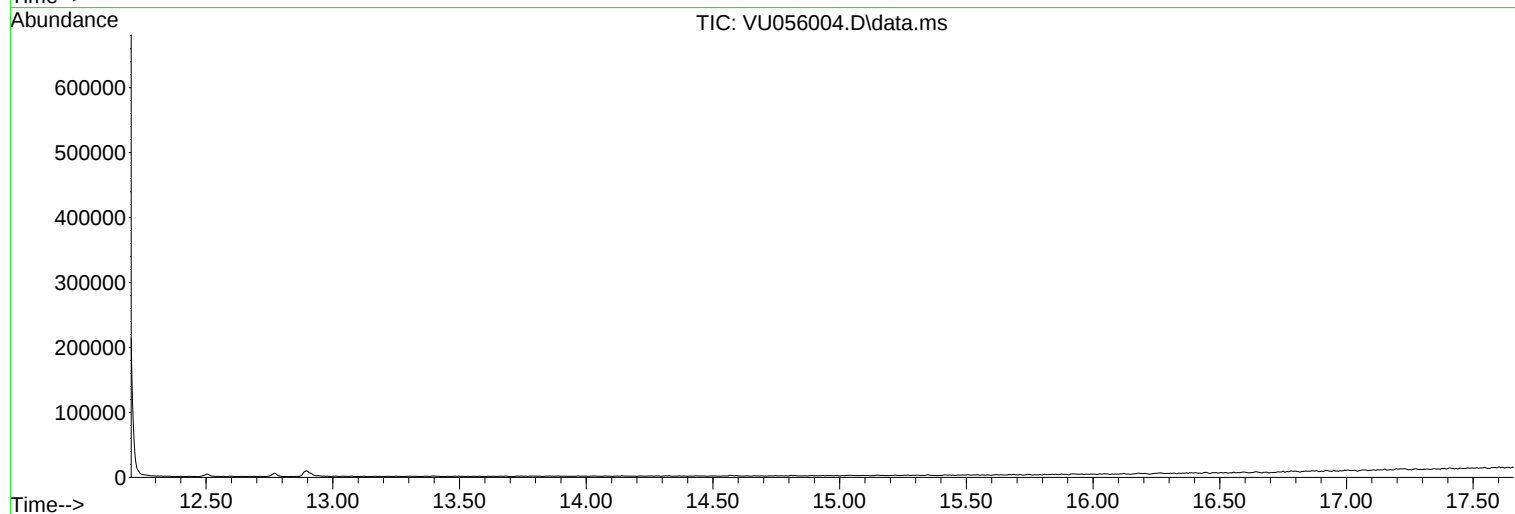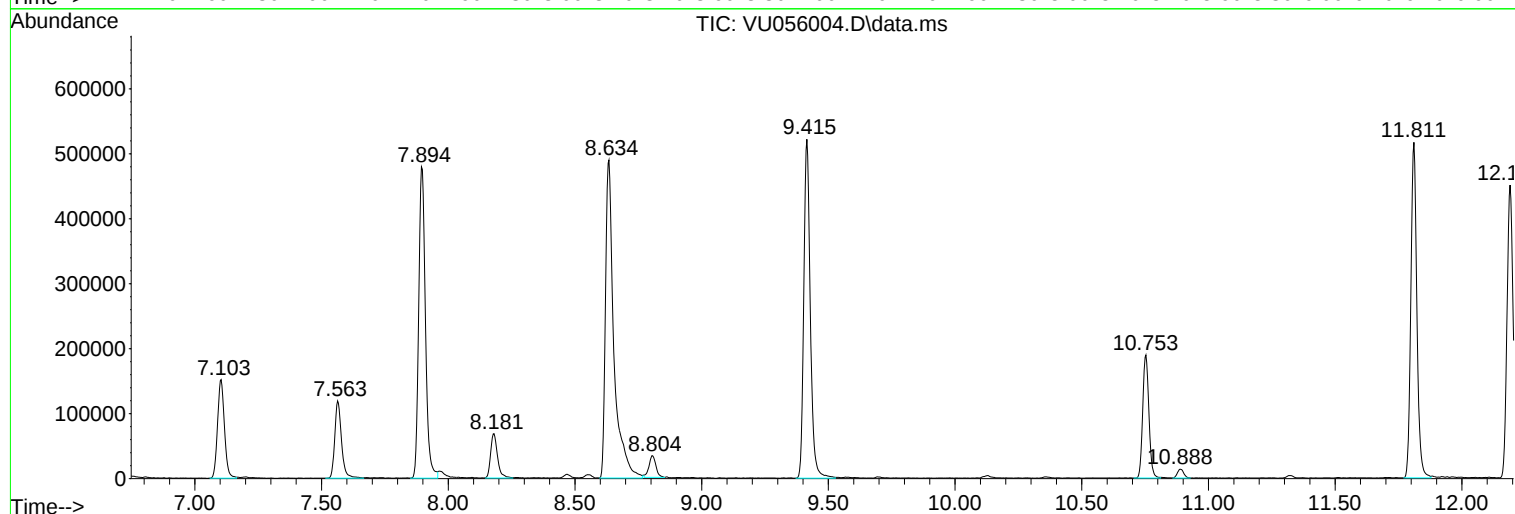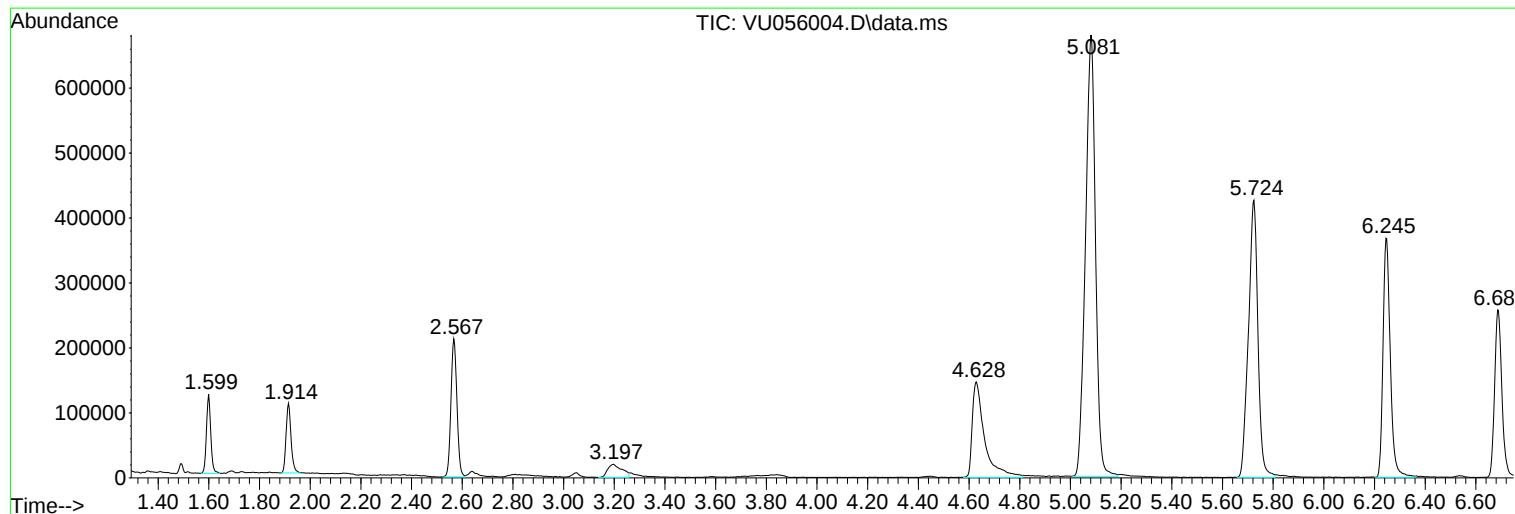

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU056004.D
Acq On : 30 Oct 2023 18:00
Operator : MD/SY
Sample : 05114-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B73










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.197	0.55 ug/L	80483	1,4-Difluorobenzene	6.248

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		3-Pentanol	88	C5H12O	000584-02-1	40
2		L-Threonine, O-methyl-, methyl e...	147	C6H13NO3	1000452-62-7	40
3		2-Propanol, 2-methyl-	74	C4H10O	000075-65-0	38
4		3-Hexanol	102	C6H14O	000623-37-0	36
5		1-Butanol, 3-methoxy-	104	C5H12O2	002517-43-3	33

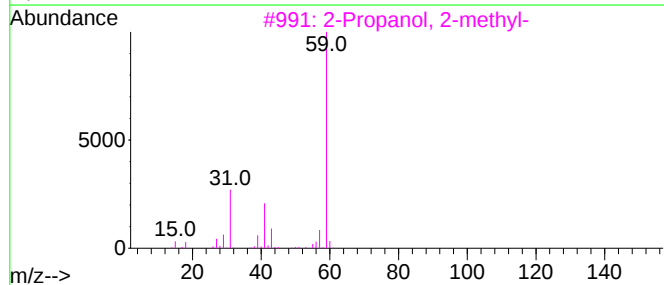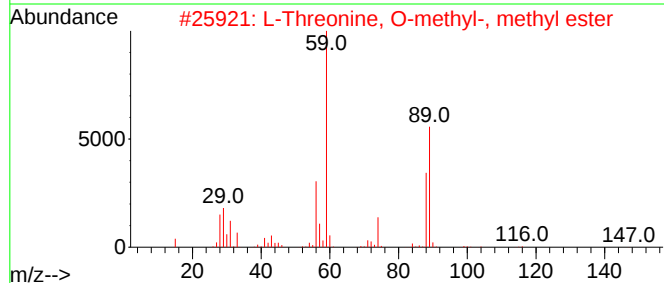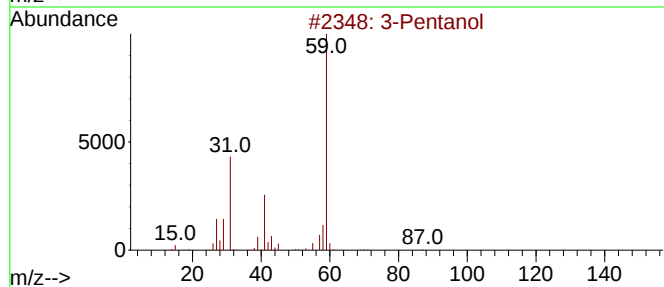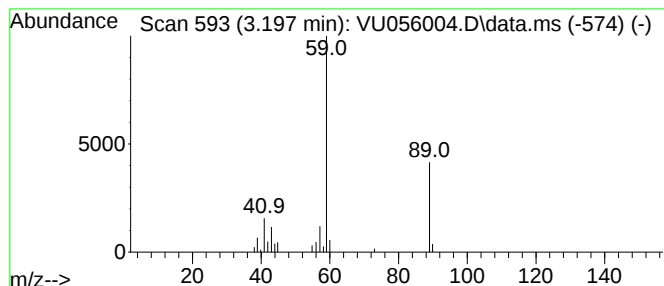

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU056004.D
Acq On : 30 Oct 2023 18:00
Operator : MD/SY
Sample : 05114-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.197	0.6	ug/L	80483	1	6.248	737726	5.0