


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103023\
Data File : VU055986.D
Acq On : 30 Oct 2023 08:26
Operator : MD/SY
Sample : BFB061
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB061

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Nov 01 01:09:14 2023

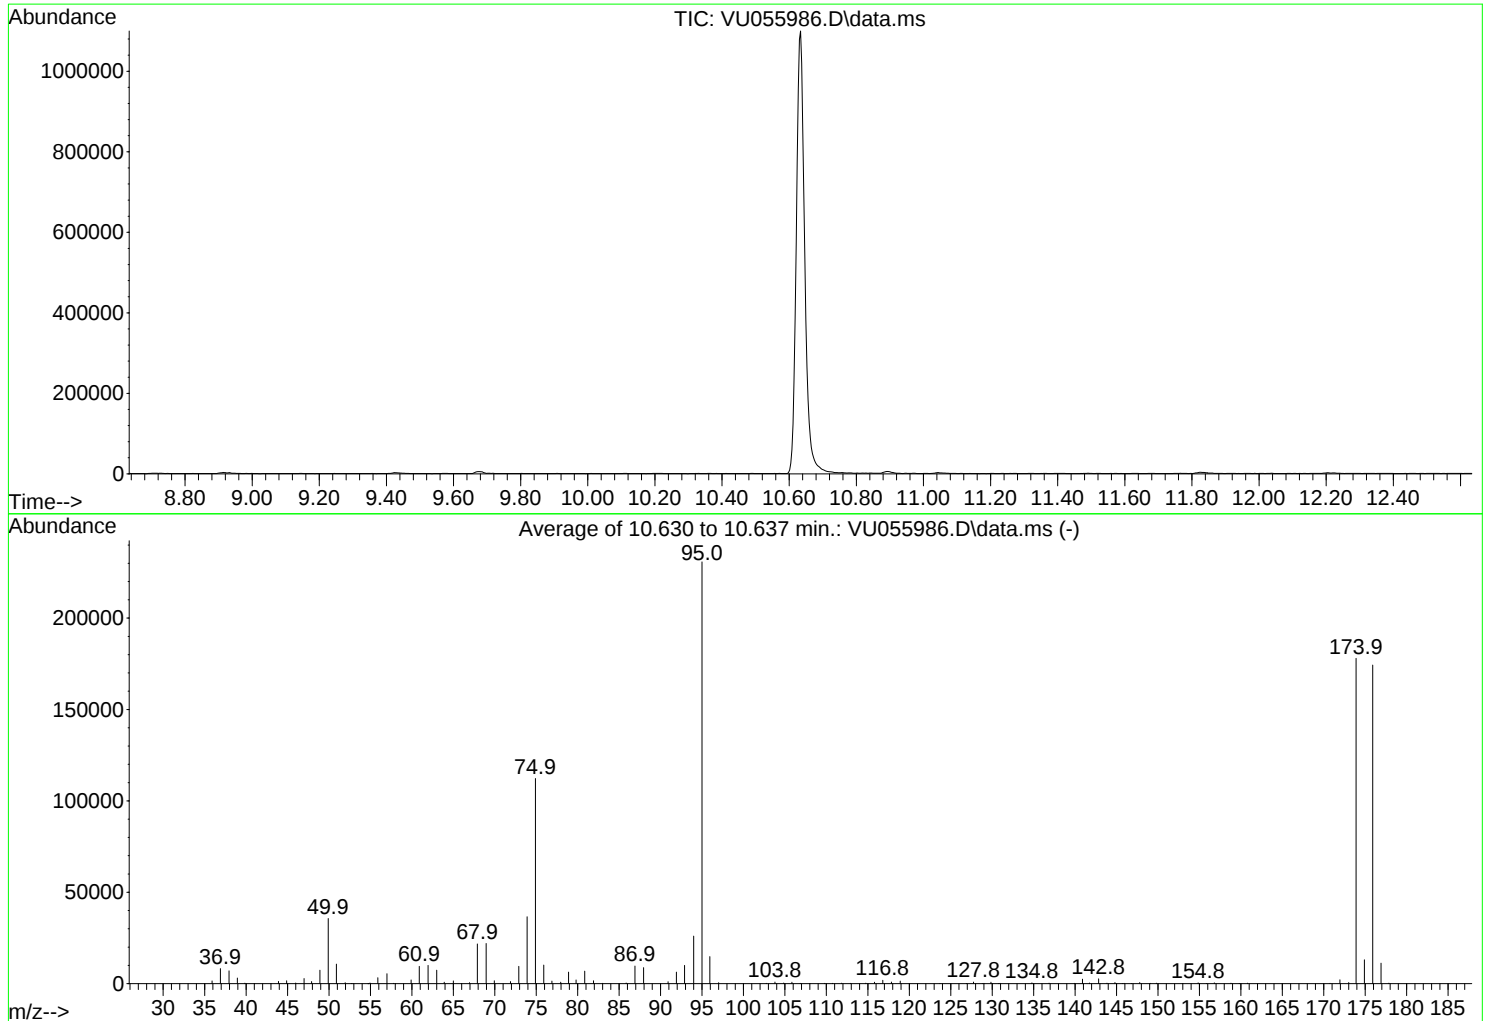

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	35648	PASS
75	95	30	80	48.7	112277	PASS
95	95	100	100	100.0	230784	PASS
96	95	5	9	6.4	14813	PASS
173	174	0.00	2	0.3	580	PASS
174	95	50	120	77.1	177941	PASS
175	174	5	9	7.3	13075	PASS
176	174	95	101	97.9	174293	PASS
177	176	5	9	6.4	11191	PASS

Scan 2891 (10.585 min): VU055986.D\data.ms
BFB061

m/z	Abundance
39.80	266.0
43.90	580.0
54.80	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.90	1523.0
36.90	8666.0
37.90	6889.0
39.00	3317.0
40.00	456.0
43.00	134.0
43.90	1809.0
44.90	1797.0
46.00	285.0
47.00	2941.0
47.90	1206.0
48.90	7759.0
49.90	36792.0
50.90	10912.0
51.90	536.0
52.70	155.0
54.90	343.0
55.90	3157.0
57.00	5755.0
57.80	271.0
59.90	2018.0
60.90	10007.0
61.90	10007.0
63.00	7700.0
63.90	951.0
65.00	1439.0
66.10	117.0
67.00	545.0
67.90	22384.0
69.00	22544.0
69.90	1817.0
71.90	1076.0
72.90	9347.0
73.90	37768.0
74.90	114040.0
75.90	10452.0
76.90	1425.0
77.90	869.0
78.90	6426.0
79.80	1974.0
80.90	7019.0
81.90	1482.0
83.00	242.0
85.90	359.0
86.90	10184.0
87.90	8717.0
90.90	982.0
91.90	6463.0
92.90	10034.0
94.00	27160.0
95.00	233920.0
96.00	15542.0
97.00	526.0
102.80	189.0
103.80	872.0
104.80	301.0
105.90	722.0
106.90	256.0
108.00	135.0
109.80	233.0
110.80	156.0
111.80	253.0
112.90	236.0
114.80	203.0
115.80	786.0
116.80	1816.0
117.90	766.0
118.90	1375.0
127.80	808.0
128.80	389.0
129.80	762.0
130.80	308.0
134.80	355.0
136.80	326.0
139.90	155.0
140.90	2265.0
141.70	338.0
142.90	2582.0
143.80	329.0
144.80	671.0
145.70	229.0
146.80	122.0
147.80	604.0
149.10	123.0
149.80	343.0
153.00	117.0
154.80	368.0
155.80	107.0
156.80	340.0
158.80	205.0
160.70	238.0
170.80	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

172.00	2071.0
173.90	177344.0
174.90	13298.0
175.90	173568.0
176.90	11313.0
177.80	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.90	1592.0
36.90	8345.0
38.00	7120.0
39.00	3175.0
39.90	519.0
41.00	105.0
43.00	141.0
43.90	1820.0
44.90	1658.0
46.00	401.0
47.00	2953.0
47.90	1128.0
48.90	7556.0
49.90	36608.0
50.90	10954.0
51.90	514.0
52.90	113.0
55.00	367.0
55.90	3357.0
57.00	5529.0
57.80	228.0
59.90	2052.0
60.90	9772.0
61.90	10312.0
63.00	7562.0
63.90	821.0
65.00	1562.0
66.00	108.0
66.90	589.0
67.90	22392.0
69.00	22504.0
69.90	1665.0
71.90	1202.0
72.90	9846.0
73.90	37632.0
74.90	116344.0
75.90	10628.0
76.90	1430.0
77.90	793.0
78.90	6543.0
79.80	2037.0
80.90	7150.0
81.90	1641.0
83.00	216.0
85.80	354.0
86.90	9756.0
87.90	9051.0
90.90	1102.0
91.90	6500.0
92.90	10179.0
94.00	26648.0
95.00	237824.0
96.00	15262.0
97.00	571.0
102.70	173.0
103.80	886.0
104.80	323.0
105.80	842.0
106.90	229.0
108.00	110.0
109.80	232.0
110.80	189.0
111.80	238.0
112.90	183.0
114.70	235.0
115.80	828.0
116.80	1940.0
117.90	855.0
118.90	1423.0
123.70	105.0
126.90	103.0
127.70	873.0
129.00	340.0
129.80	839.0
131.00	288.0
134.80	434.0
136.80	290.0
139.90	194.0
140.90	2526.0
141.80	355.0
142.80	2755.0
143.90	274.0
144.80	661.0
145.90	264.0
146.80	108.0
147.80	585.0
149.10	137.0
149.80	308.0
153.00	125.0
154.80	477.0
155.90	134.0
156.80	429.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

158.80	276.0
159.80	125.0
160.80	248.0
170.70	163.0
171.90	2094.0
173.90	183936.0
174.90	13480.0
175.90	180160.0
176.90	11623.0
177.80	264.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.90	1450.0
36.90	7656.0
38.00	6906.0
38.90	2772.0
39.90	560.0
41.00	103.0
43.00	119.0
43.90	1739.0
44.90	1280.0
46.00	377.0
47.00	2409.0
47.90	1020.0
48.90	6761.0
49.90	33544.0
50.90	10062.0
52.00	447.0
52.90	105.0
54.70	343.0
55.00	371.0
55.90	3179.0
57.00	5064.0
58.00	200.0
59.90	1935.0
60.90	8608.0
62.00	9604.0
63.00	6708.0
63.90	737.0
65.00	1377.0
65.90	116.0
66.90	582.0
67.90	20376.0
68.90	20872.0
70.00	1361.0
71.90	1184.0
72.90	9302.0
73.90	34344.0
74.90	106448.0
75.90	9455.0
76.90	1330.0
78.00	686.0
78.90	5909.0
79.80	1921.0
80.80	6378.0
81.90	1607.0
83.00	181.0
85.80	316.0
86.90	8842.0
88.00	8392.0
90.90	1066.0
91.90	5845.0
92.90	9648.0
94.00	24072.0
95.00	220608.0
95.90	13636.0
97.00	555.0
102.70	103.0
103.80	899.0
104.90	349.0
105.80	953.0
106.80	172.0
109.80	159.0
110.70	193.0
111.90	183.0
112.80	120.0
114.70	240.0
115.80	767.0
116.80	1767.0
117.80	925.0
118.90	1297.0
123.70	111.0
126.90	145.0
127.70	921.0
129.00	313.0
129.90	811.0
130.90	292.0
134.80	471.0
136.90	229.0
139.90	147.0
140.90	2554.0
141.80	355.0
142.80	2485.0
143.90	188.0
144.80	536.0
145.90	300.0
147.80	605.0
149.00	157.0
149.80	240.0
153.00	152.0
154.90	451.0
155.90	127.0
156.80	483.0
158.80	339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

159.80	151.0
160.90	258.0
170.80	181.0
171.90	2042.0
173.00	1741.0
173.90	172544.0
174.90	12446.0
175.90	169152.0
176.90	10636.0
177.90	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061