

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061295.D
 Acq On : 30 Oct 2024 10:47
 Operator : MD/SY
 Sample : VU1030WBL01
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Oct 31 22:50:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 31 22:49:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	244333	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	226543	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	104651	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	82671	48.172	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.340%
7) Chloroethane-d5	1.904	69	74000	49.301	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	98.600%
11) 1,1-Dichloroethene-d2	2.560	63	123690	39.173	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.340%
21) 2-Butanone-d5	4.612	46	138991	98.188	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.190%
24) Chloroform-d	5.052	84	179945	49.543	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.080%
26) 1,2-Dichloroethane-d4	5.692	65	118797	51.382	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.760%
32) Benzene-d6	5.718	84	377037	51.978	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.960%
36) 1,2-Dichloropropane-d6	6.679	67	117899	53.115	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.240%
41) Toluene-d8	7.891	98	344463	51.007	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.020%
43) trans-1,3-Dichloroprop...	8.174	79	56157	50.606	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.220%
47) 2-Hexanone-d5	8.624	63	109356	97.381	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.380%
56) 1,1,2,2-Tetrachloroeth...	10.746	84	170210	48.722	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.440%
66) 1,2-Dichlorobenzene-d4	12.187	152	119481	51.574	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.140%
Target Compounds						
39) cis-1,3-Dichloropropene	7.557	75	3717	1.365	ug/L	Qvalue # 15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061295.D
Acq On : 30 Oct 2024 10:47
Operator : MD/SY
Sample : VU1030WBL01
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Oct 31 22:50:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 31 22:49:53 2024
Response via : Initial Calibration

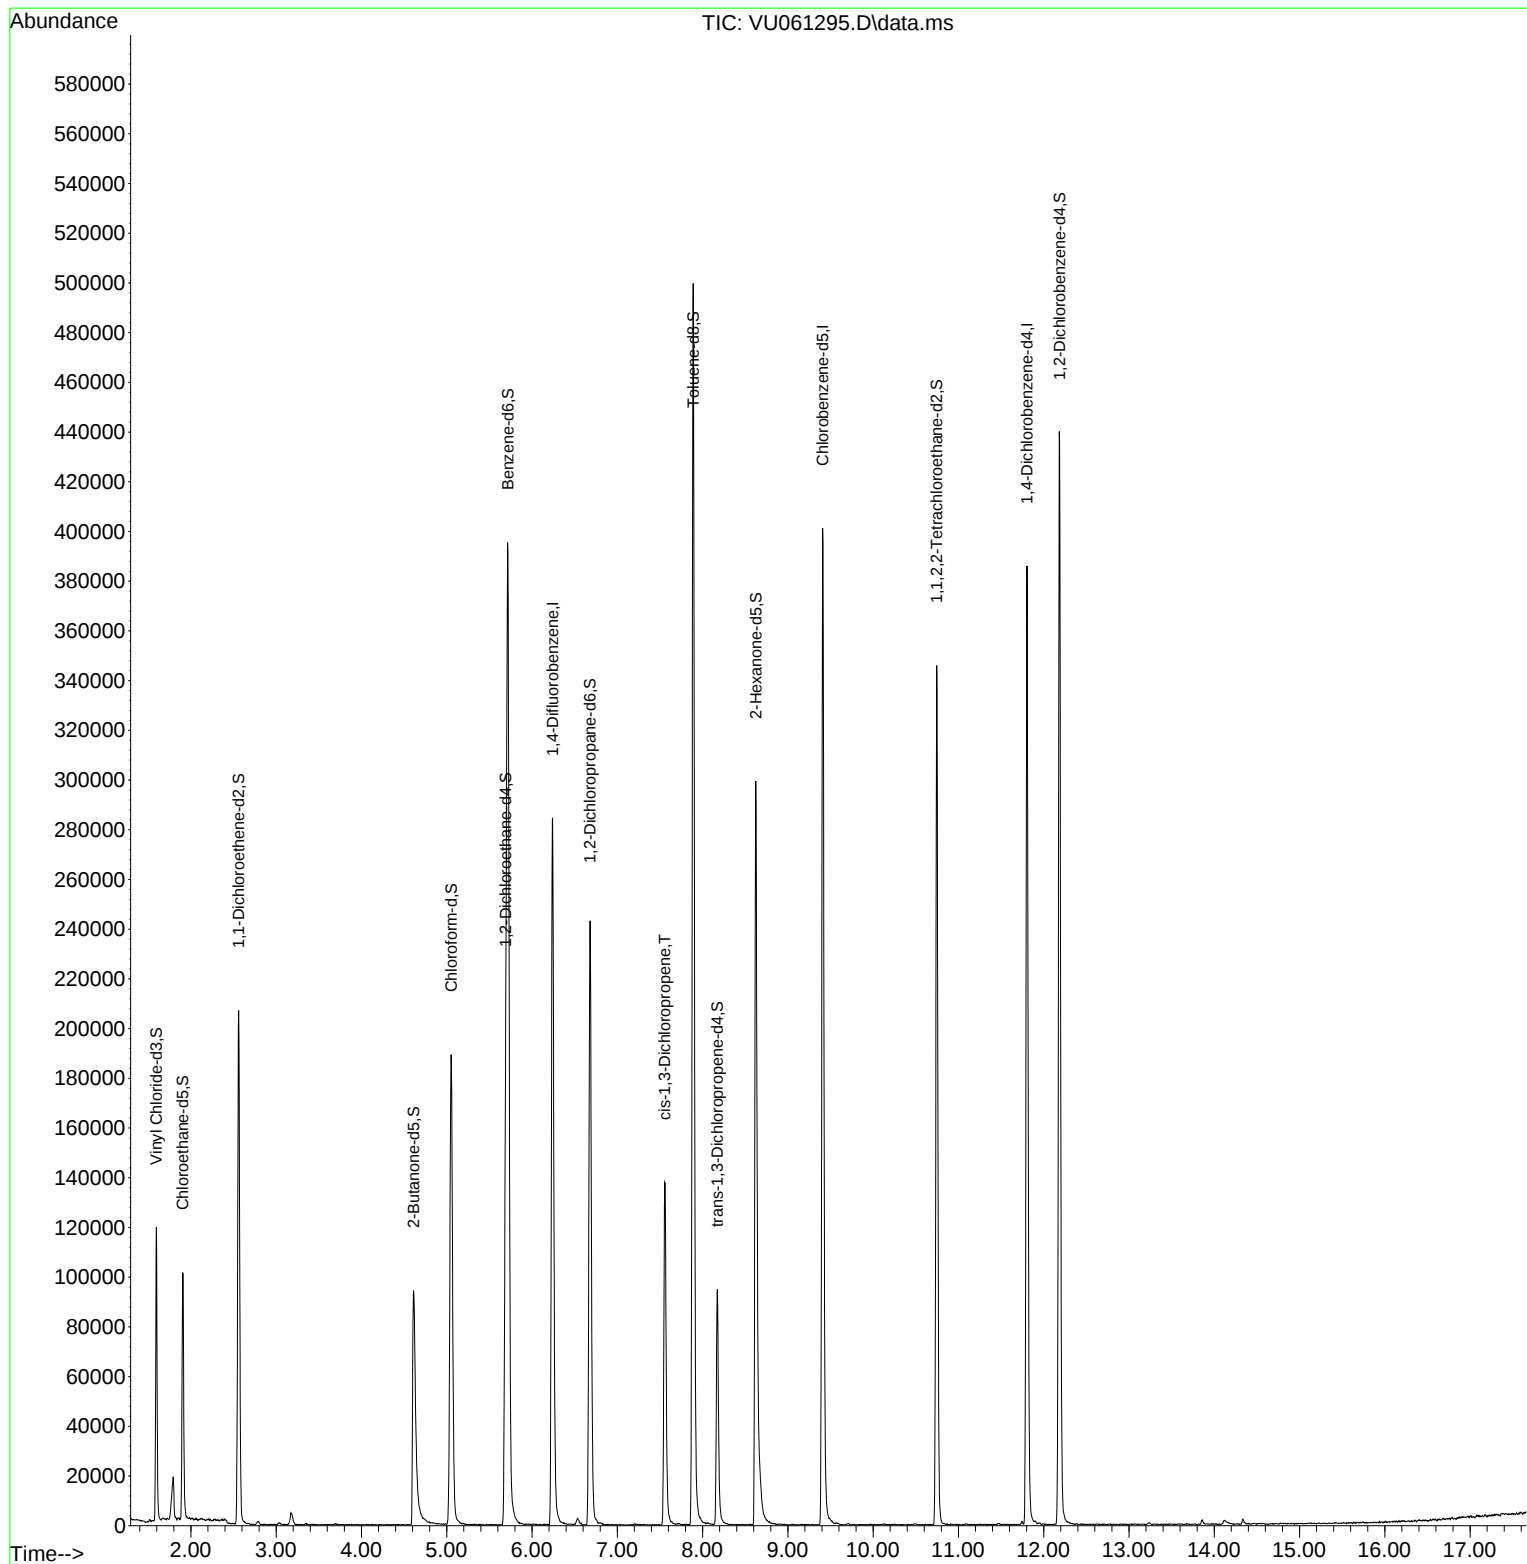

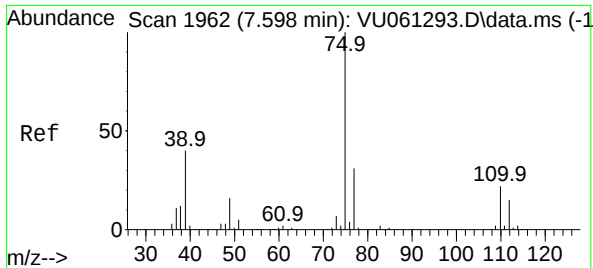

#39
cis-1,3-Dichloropropene
Concen: 1.365 ug/L
RT: 7.557 min Scan# 1949
Delta R.T. -0.042 min
Lab File: VU061295.D
Acq: 30 Oct 2024 10:47

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 75 Resp: 3717
Ion Ratio Lower Upper
75 100
77 79.3 22.5 41.7#

