

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061301.D
 Acq On : 30 Oct 2024 14:43
 Operator : MD/SY
 Sample : P4581-18
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Oct 31 22:51:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 31 22:49:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	252487	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	229298	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	104878	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	74448	41.980	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.960%		
7) Chloroethane-d5	1.904	69	65407	42.169	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.340%		
11) 1,1-Dichloroethene-d2	2.560	63	109694	33.618	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.240%		
21) 2-Butanone-d5	4.612	46	121141	82.814	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.810%		
24) Chloroform-d	5.052	84	154955	41.285	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.560%		
26) 1,2-Dichloroethane-d4	5.692	65	104849	43.884	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.760%		
32) Benzene-d6	5.718	84	323694	44.088	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.180%		
36) 1,2-Dichloropropane-d6	6.679	67	101067	44.985	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.960%		
41) Toluene-d8	7.891	98	293857	42.991	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.980%		
43) trans-1,3-Dichloroprop...	8.174	79	46703	41.581	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.160%		
47) 2-Hexanone-d5	8.624	63	91577	80.569	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.570%		
56) 1,1,2,2-Tetrachloroeth...	10.746	84	143202	40.498	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	81.000%		
66) 1,2-Dichlorobenzene-d4	12.187	152	100439	43.261	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.520%		
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.804	75	13510	6.070	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061301.D
Acq On : 30 Oct 2024 14:43
Operator : MD/SY
Sample : P4581-18
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Oct 31 22:51:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 31 22:49:53 2024
Response via : Initial Calibration

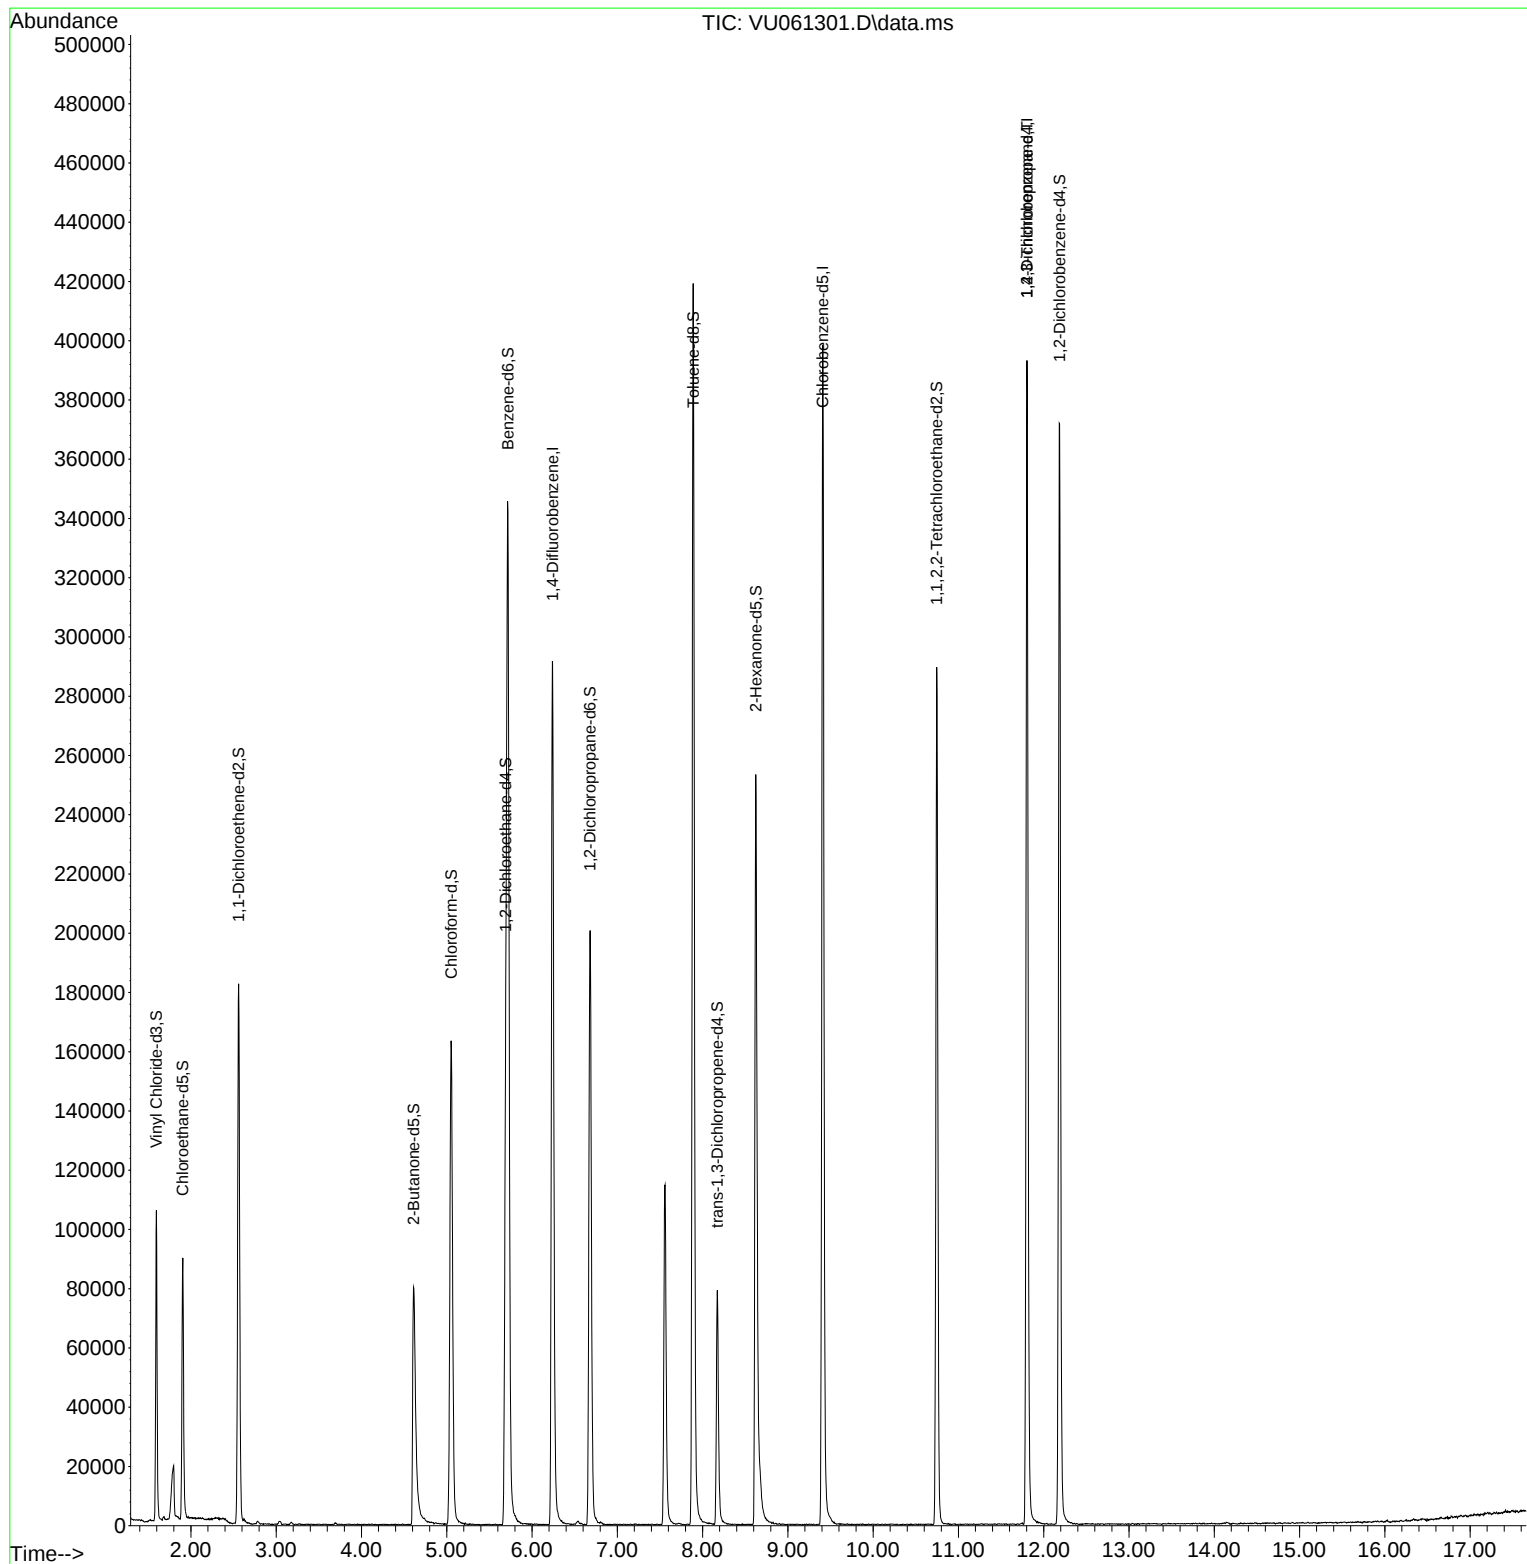

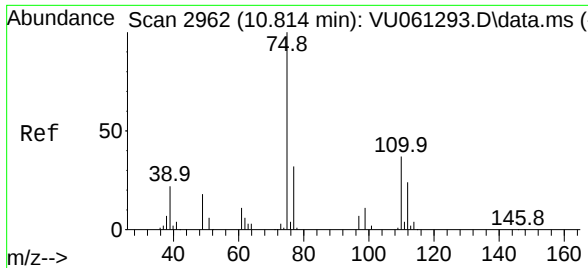

#60
1,2,3-Trichloropropane
Concen: 6.070 ug/L
RT: 11.804 min Scan# 31
Delta R.T. 0.990 min
Lab File: VU061301.D
Acq: 30 Oct 2024 14:43

Instrument :
MSVOA_U
ClientSampleId :

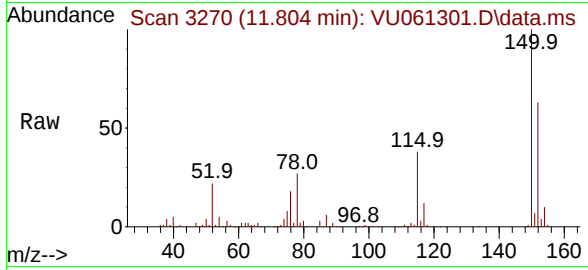

Tgt Ion: 75 Resp: 13510
Ion Ratio Lower Upper
75 100
77 31.4 25.5 38.3
110 2.1 29.8 44.6#

