

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061298.D
 Acq On : 30 Oct 2024 13:09
 Operator : MD/SY
 Sample : P4582-10
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4EC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

Signal : TIC: VU061298.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rBV	111532	126611	12.97%	1.689%
2	1.782	139	153	154	rBV2	18767	33389	3.42%	0.445%
3	1.904	182	191	211	rVB	87823	124781	12.79%	1.665%
4	2.560	382	395	406	rBV	192458	316932	32.48%	4.228%
5	2.618	406	413	430	rVB	23842	43934	4.50%	0.586%
6	2.750	446	454	461	rBV3	4311	8078	0.83%	0.108%
7	3.010	532	535	537	rBV	283	177	0.02%	0.002%
8	3.178	577	587	593	rBV3	955	1711	0.18%	0.023%
9	3.412	656	660	662	rBV	309	213	0.02%	0.003%
10	3.493	682	685	689	rBV	235	194	0.02%	0.003%
11	3.563	703	707	709	rBV	215	198	0.02%	0.003%
12	3.650	731	734	742	rVB2	215	193	0.02%	0.003%
13	3.686	742	745	746	rBV	579	261	0.03%	0.003%
14	3.788	774	777	781	rVB2	217	204	0.02%	0.003%
15	3.821	781	787	793	rVB2	249	346	0.04%	0.005%
16	3.898	804	811	813	rBV	280	335	0.03%	0.004%
17	4.055	854	860	861	rBV	211	203	0.02%	0.003%
18	4.210	903	908	912	rBV2	218	218	0.02%	0.003%
19	4.518	1002	1004	1011	rVB2	339	299	0.03%	0.004%
20	4.557	1011	1016	1019	rBV	219	185	0.02%	0.002%
21	4.608	1022	1032	1064	rBV	83441	210326	21.55%	2.806%
22	5.052	1155	1170	1193	rBV	172866	383482	39.30%	5.116%
23	5.190	1210	1213	1216	rVB3	372	270	0.03%	0.004%
24	5.245	1228	1230	1235	rVB3	256	178	0.02%	0.002%
25	5.332	1253	1257	1260	rBV	199	200	0.02%	0.003%
26	5.409	1273	1281	1283	rBV	307	369	0.04%	0.005%
27	5.534	1313	1320	1323	rVB2	275	385	0.04%	0.005%
28	5.557	1323	1327	1330	rBV2	249	217	0.02%	0.003%
29	5.714	1355	1376	1402	rBV2	356150	975820	100.00%	13.018%
30	6.068	1483	1486	1492	rVB2	325	281	0.03%	0.004%
31	6.238	1527	1539	1566	rBV	296181	577269	59.16%	7.701%
32	6.531	1623	1630	1634	rBV2	1374	1733	0.18%	0.023%
33	6.679	1657	1676	1708	rBV	216326	430325	44.10%	5.741%
34	6.804	1713	1715	1719	rBV4	361	254	0.03%	0.003%
35	6.898	1741	1744	1750	rVV4	834	890	0.09%	0.012%
36	6.943	1755	1758	1761	rVB3	323	207	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061298.D
 Acq On : 30 Oct 2024 13:09
 Operator : MD/SY
 Sample : P4582-10
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4EC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

37	7.039	1785	1788	1791	rBV2	243	188	0.02%	0.003%
38	7.094	1802	1805	1809	rVB2	237	201	0.02%	0.003%
39	7.197	1830	1837	1841	rBV2	404	458	0.05%	0.006%
40	7.222	1841	1845	1849	rBV2	217	197	0.02%	0.003%
41	7.367	1887	1890	1895	rVB2	202	189	0.02%	0.003%
42	7.412	1900	1904	1908	rBV2	226	210	0.02%	0.003%
43	7.489	1924	1928	1932	rBV2	208	215	0.02%	0.003%
44	7.557	1938	1949	1975	rBV	123670	224535	23.01%	2.995%
45	7.891	2040	2053	2083	rBV	439981	797726	81.75%	10.642%
46	8.113	2120	2122	2130	rVB2	531	505	0.05%	0.007%
47	8.171	2130	2140	2165	rBV	83165	148830	15.25%	1.985%
48	8.354	2193	2197	2198	rBV	297	212	0.02%	0.003%
49	8.483	2234	2237	2239	rBV2	233	178	0.02%	0.002%
50	8.544	2251	2256	2258	rBV2	206	190	0.02%	0.003%
51	8.624	2270	2281	2321	rBV	263911	512643	52.53%	6.839%
52	8.788	2325	2332	2343	rVB7	5534	10618	1.09%	0.142%
53	9.013	2398	2402	2408	rVB2	278	278	0.03%	0.004%
54	9.094	2422	2427	2429	rBV	251	222	0.02%	0.003%
55	9.155	2442	2446	2449	rBV2	346	292	0.03%	0.004%
56	9.264	2474	2480	2484	rBV2	388	433	0.04%	0.006%
57	9.409	2513	2525	2560	rBV	412587	713456	73.11%	9.518%
58	9.566	2570	2574	2576	rBV3	370	341	0.03%	0.005%
59	9.698	2610	2615	2619	rVV3	193	212	0.02%	0.003%
60	9.807	2645	2649	2652	rBV	249	193	0.02%	0.003%
61	10.145	2748	2754	2759	rBV3	361	457	0.05%	0.006%
62	10.190	2762	2768	2772	rBV2	253	340	0.03%	0.005%
63	10.258	2783	2789	2793	rBV3	488	653	0.07%	0.009%
64	10.312	2803	2806	2812	rVB2	180	180	0.02%	0.002%
65	10.573	2884	2887	2889	rBV2	387	232	0.02%	0.003%
66	10.586	2889	2891	2896	rVB2	568	392	0.04%	0.005%
67	10.624	2896	2903	2906	rBV2	234	333	0.03%	0.004%
68	10.746	2928	2941	2964	rBV	304338	496509	50.88%	6.624%
69	10.852	2970	2974	2983	rVB3	473	673	0.07%	0.009%
70	11.094	3045	3049	3053	rBV3	258	197	0.02%	0.003%
71	11.322	3117	3120	3125	rBV	216	225	0.02%	0.003%
72	11.405	3143	3146	3151	rVB	229	226	0.02%	0.003%
73	11.428	3151	3153	3157	rBV	227	177	0.02%	0.002%
74	11.467	3162	3165	3167	rBV	295	195	0.02%	0.003%
75	11.496	3172	3174	3179	rBV	317	282	0.03%	0.004%
76	11.537	3183	3187	3189	rVB	264	194	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061298.D
 Acq On : 30 Oct 2024 13:09
 Operator : MD/SY
 Sample : P4582-10
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4EC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

77	11.660	3222	3225	3232	rBV2	155	198	0.02%	0.003%
78	11.701	3235	3238	3240	rBV	362	240	0.02%	0.003%
79	11.746	3249	3252	3255	rVB4	559	331	0.03%	0.004%
80	11.804	3258	3270	3307	rBV	396958	660223	67.66%	8.808%
81	12.081	3346	3356	3372	rBV5	2508	6951	0.71%	0.093%
82	12.184	3376	3388	3414	rVV	391627	666926	68.35%	8.897%
83	12.286	3418	3420	3427	rVB5	389	380	0.04%	0.005%
84	12.537	3491	3498	3502	rBV4	951	1251	0.13%	0.017%
85	12.852	3593	3596	3601	rVB5	635	483	0.05%	0.006%
86	13.055	3654	3659	3661	rBV2	379	319	0.03%	0.004%
87	13.299	3732	3735	3738	rBV2	234	200	0.02%	0.003%
88	13.357	3746	3753	3757	rBV2	284	416	0.04%	0.006%
89	13.492	3792	3795	3801	rVB2	260	268	0.03%	0.004%
90	13.540	3807	3810	3814	rBV2	239	266	0.03%	0.004%
91	13.605	3827	3830	3833	rBV	242	180	0.02%	0.002%
92	13.730	3866	3869	3873	rVB	379	282	0.03%	0.004%
93	14.119	3987	3990	3993	rBV2	391	425	0.04%	0.006%
94	14.643	4150	4153	4156	rBV2	223	179	0.02%	0.002%
95	14.865	4219	4222	4226	rBV2	302	221	0.02%	0.003%
96	14.888	4226	4229	4232	rBV2	303	240	0.02%	0.003%
97	15.392	4383	4386	4388	rBV2	343	232	0.02%	0.003%
98	15.855	4528	4530	4532	rBV	415	262	0.03%	0.003%
99	16.029	4582	4584	4588	rBV2	447	389	0.04%	0.005%
100	16.444	4711	4713	4717	rBV3	798	604	0.06%	0.008%

Sum of corrected areas: 7495921




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061298.D
Acq On : 30 Oct 2024 13:09
Operator : MD/SY
Sample : P4582-10
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4EC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

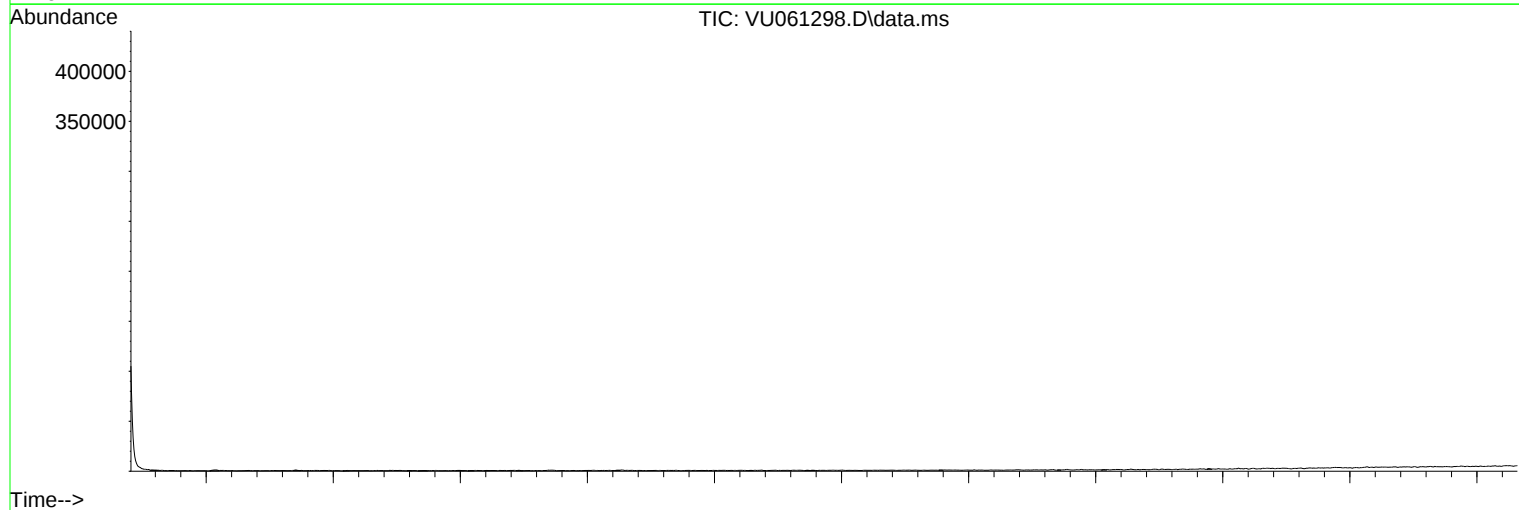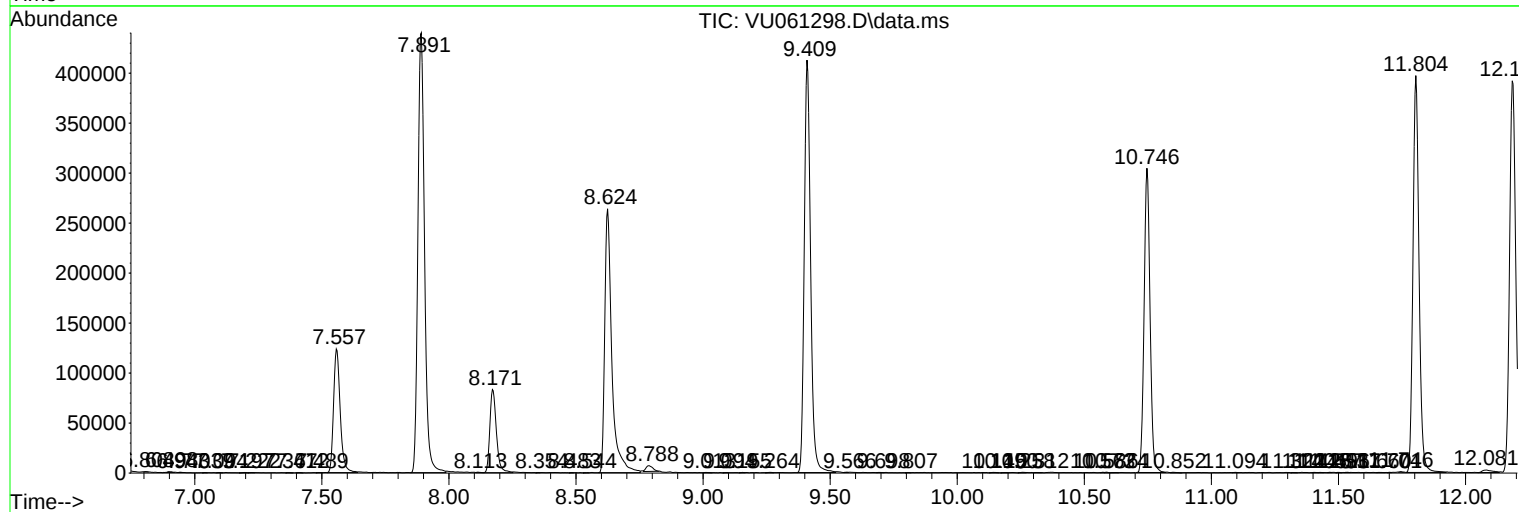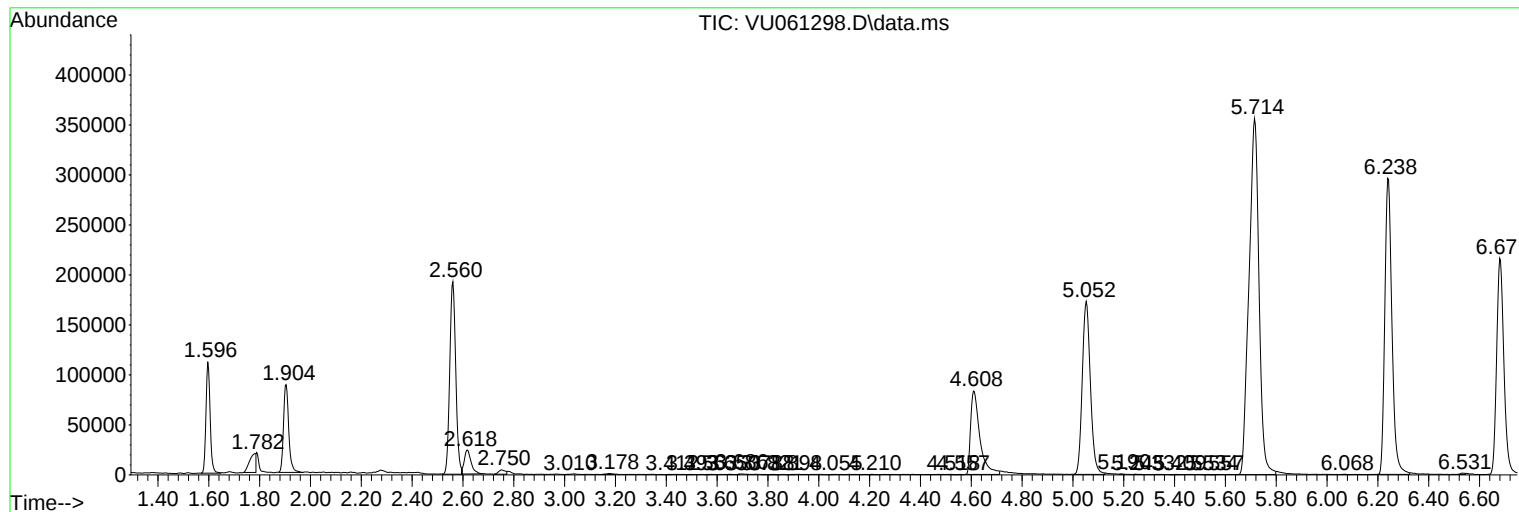

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061298.D
Acq On : 30 Oct 2024 13:09
Operator : MD/SY
Sample : P4582-10
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4EC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061298.D
Acq On : 30 Oct 2024 13:09
Operator : MD/SY
Sample : P4582-10
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4EC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------