

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061300.D
 Acq On : 30 Oct 2024 14:19
 Operator : MD/SY
 Sample : P4582-07
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

Signal : TIC: VU061300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	110	rBV	110378	125245	12.78%	1.660%
2	1.904	183	191	208	rVB	88468	119378	12.18%	1.583%
3	2.560	383	395	411	rBV	206333	337042	34.39%	4.468%
4	2.904	497	502	504	rBV2	358	327	0.03%	0.004%
5	2.949	514	516	517	rBV	256	111	0.01%	0.001%
6	3.036	537	543	553	rVB5	1342	1993	0.20%	0.026%
7	3.174	580	586	592	rBV2	830	1100	0.11%	0.015%
8	3.255	609	611	613	rBV	163	101	0.01%	0.001%
9	3.351	637	641	643	rBV2	385	325	0.03%	0.004%
10	3.422	660	663	664	rBV	131	83	0.01%	0.001%
11	3.454	671	673	675	rBV	152	105	0.01%	0.001%
12	3.496	682	686	687	rBV	165	90	0.01%	0.001%
13	3.695	744	748	751	rBV2	438	434	0.04%	0.006%
14	3.766	761	770	772	rBV2	254	379	0.04%	0.005%
15	3.869	794	802	806	rBV2	292	484	0.05%	0.006%
16	3.930	816	821	824	rBV2	263	264	0.03%	0.003%
17	4.087	867	870	877	rBV2	179	271	0.03%	0.004%
18	4.258	920	923	925	rBV2	187	110	0.01%	0.001%
19	4.274	925	928	929	rBV	204	115	0.01%	0.002%
20	4.354	950	953	954	rBV	110	79	0.01%	0.001%
21	4.476	989	991	992	rBV	158	83	0.01%	0.001%
22	4.554	1007	1015	1019	rVB2	345	496	0.05%	0.007%
23	4.579	1019	1023	1024	rBV2	262	188	0.02%	0.002%
24	4.611	1024	1033	1076	rBV	80883	206507	21.07%	2.738%
25	5.052	1155	1170	1194	rBV	170267	384757	39.25%	5.101%
26	5.261	1229	1235	1238	rBV2	142	150	0.02%	0.002%
27	5.277	1238	1240	1243	rVV2	228	113	0.01%	0.001%
28	5.390	1273	1275	1278	rVB	224	101	0.01%	0.001%
29	5.406	1278	1280	1283	rBV2	189	112	0.01%	0.001%
30	5.473	1298	1301	1302	rBV2	199	96	0.01%	0.001%
31	5.483	1302	1304	1307	rVV	227	154	0.02%	0.002%
32	5.518	1311	1315	1319	rVB2	191	204	0.02%	0.003%
33	5.547	1319	1324	1326	rBV	116	88	0.01%	0.001%
34	5.579	1330	1334	1336	rBV	114	89	0.01%	0.001%
35	5.618	1343	1346	1351	rVB2	232	188	0.02%	0.002%
36	5.718	1351	1377	1400	rBV2	357800	980175	100.00%	12.994%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061300.D
 Acq On : 30 Oct 2024 14:19
 Operator : MD/SY
 Sample : P4582-07
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

37	5.904	1433	1435	1437	rBV2	302	146	0.01%	0.002%
38	6.004	1463	1466	1472	rBV2	222	261	0.03%	0.003%
39	6.116	1499	1501	1503	rBV	158	98	0.01%	0.001%
40	6.242	1528	1540	1575	rBV	320816	621811	63.44%	8.243%
41	6.537	1625	1632	1638	rBV6	1259	2287	0.23%	0.030%
42	6.605	1651	1653	1656	rBV	139	94	0.01%	0.001%
43	6.682	1661	1677	1706	rBV	216206	426581	43.52%	5.655%
44	6.856	1728	1731	1734	rBV	228	154	0.02%	0.002%
45	6.923	1748	1752	1754	rBV2	396	342	0.03%	0.005%
46	6.949	1758	1760	1764	rBV2	181	172	0.02%	0.002%
47	6.997	1772	1775	1782	rBV2	206	250	0.03%	0.003%
48	7.033	1782	1786	1792	rVB2	208	204	0.02%	0.003%
49	7.087	1801	1803	1806	rBV	177	107	0.01%	0.001%
50	7.177	1827	1831	1833	rBV	165	103	0.01%	0.001%
51	7.206	1837	1840	1843	rBV2	291	219	0.02%	0.003%
52	7.258	1854	1856	1860	rBV	188	127	0.01%	0.002%
53	7.280	1860	1863	1866	rVB	141	124	0.01%	0.002%
54	7.299	1866	1869	1872	rBV2	275	170	0.02%	0.002%
55	7.341	1878	1882	1886	rBV	230	154	0.02%	0.002%
56	7.367	1886	1890	1891	rBV	157	102	0.01%	0.001%
57	7.435	1908	1911	1913	rBV	360	269	0.03%	0.004%
58	7.560	1938	1950	1976	rBV	124480	228480	23.31%	3.029%
59	7.820	2028	2031	2035	rBV2	254	226	0.02%	0.003%
60	7.891	2040	2053	2087	rBV	458900	806280	82.26%	10.689%
61	8.174	2130	2141	2163	rBV	84635	149138	15.22%	1.977%
62	8.367	2199	2201	2203	rVB	236	109	0.01%	0.001%
63	8.383	2204	2206	2215	rVB2	195	263	0.03%	0.003%
64	8.422	2215	2218	2220	rBV2	190	139	0.01%	0.002%
65	8.624	2271	2281	2317	rBV	253163	495041	50.51%	6.563%
66	9.055	2411	2415	2418	rBV2	178	165	0.02%	0.002%
67	9.155	2443	2446	2449	rBV	211	155	0.02%	0.002%
68	9.238	2467	2472	2474	rBV2	174	166	0.02%	0.002%
69	9.277	2482	2484	2487	rBV2	171	126	0.01%	0.002%
70	9.412	2514	2526	2553	rBV	432203	757511	77.28%	10.042%
71	9.663	2601	2604	2606	rBV	344	262	0.03%	0.003%
72	10.106	2739	2742	2744	rVB3	266	165	0.02%	0.002%
73	10.139	2747	2752	2758	rVB3	393	405	0.04%	0.005%
74	10.171	2759	2762	2766	rBV2	197	186	0.02%	0.002%
75	10.238	2780	2783	2788	rBV2	351	296	0.03%	0.004%
76	10.380	2825	2827	2830	rBV	215	139	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
 Data File : VU061300.D
 Acq On : 30 Oct 2024 14:19
 Operator : MD/SY
 Sample : P4582-07
 Misc : 5mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
 Title : VOC Analysis

77	10.444	2843	2847	2848	rBV	148	109	0.01%	0.001%
78	10.749	2929	2942	2961	rBV	300764	489255	49.92%	6.486%
79	10.885	2980	2984	2991	rBV3	382	397	0.04%	0.005%
80	11.013	3021	3024	3025	rBV2	189	104	0.01%	0.001%
81	11.081	3040	3045	3046	rBV2	184	179	0.02%	0.002%
82	11.161	3068	3070	3071	rBV	186	82	0.01%	0.001%
83	11.341	3124	3126	3129	rBV2	162	81	0.01%	0.001%
84	11.454	3157	3161	3164	rBV2	157	152	0.02%	0.002%
85	11.579	3197	3200	3203	rBV2	205	143	0.01%	0.002%
86	11.701	3235	3238	3240	rBV	162	110	0.01%	0.001%
87	11.753	3247	3254	3258	rBV4	927	1055	0.11%	0.014%
88	11.804	3258	3270	3309	rVV	428651	716690	73.12%	9.501%
89	12.003	3327	3332	3335	rBV4	472	501	0.05%	0.007%
90	12.084	3355	3357	3360	rBV2	489	340	0.03%	0.005%
91	12.135	3370	3373	3375	rBV	295	240	0.02%	0.003%
92	12.187	3377	3389	3413	rVV	399213	676820	69.05%	8.972%
93	12.573	3505	3509	3515	rBV2	286	354	0.04%	0.005%
94	12.991	3634	3639	3641	rBV2	275	278	0.03%	0.004%
95	13.093	3668	3671	3674	rVB2	360	217	0.02%	0.003%
96	13.232	3712	3714	3720	rBV	344	285	0.03%	0.004%
97	13.492	3792	3795	3797	rBV2	239	175	0.02%	0.002%
98	13.859	3906	3909	3910	rBV2	402	214	0.02%	0.003%
99	14.354	4059	4063	4065	rBV2	517	383	0.04%	0.005%
100	14.688	4164	4167	4172	rBV2	497	545	0.06%	0.007%

Sum of corrected areas: 7543273




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061300.D
Acq On : 30 Oct 2024 14:19
Operator : MD/SY
Sample : P4582-07
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

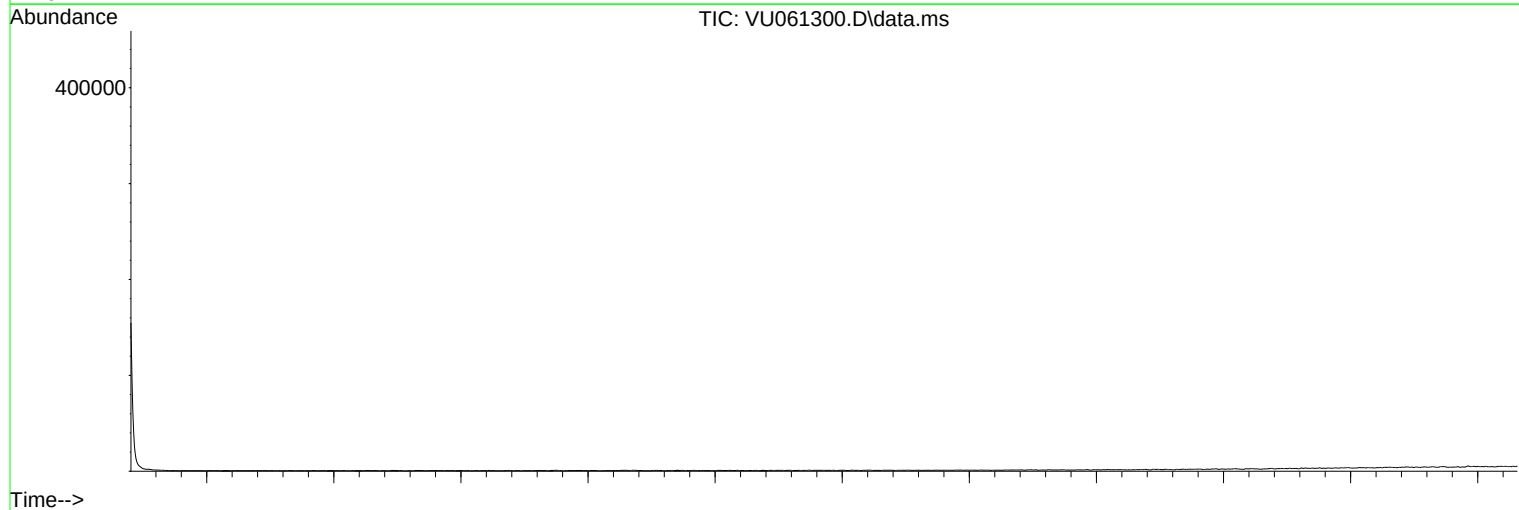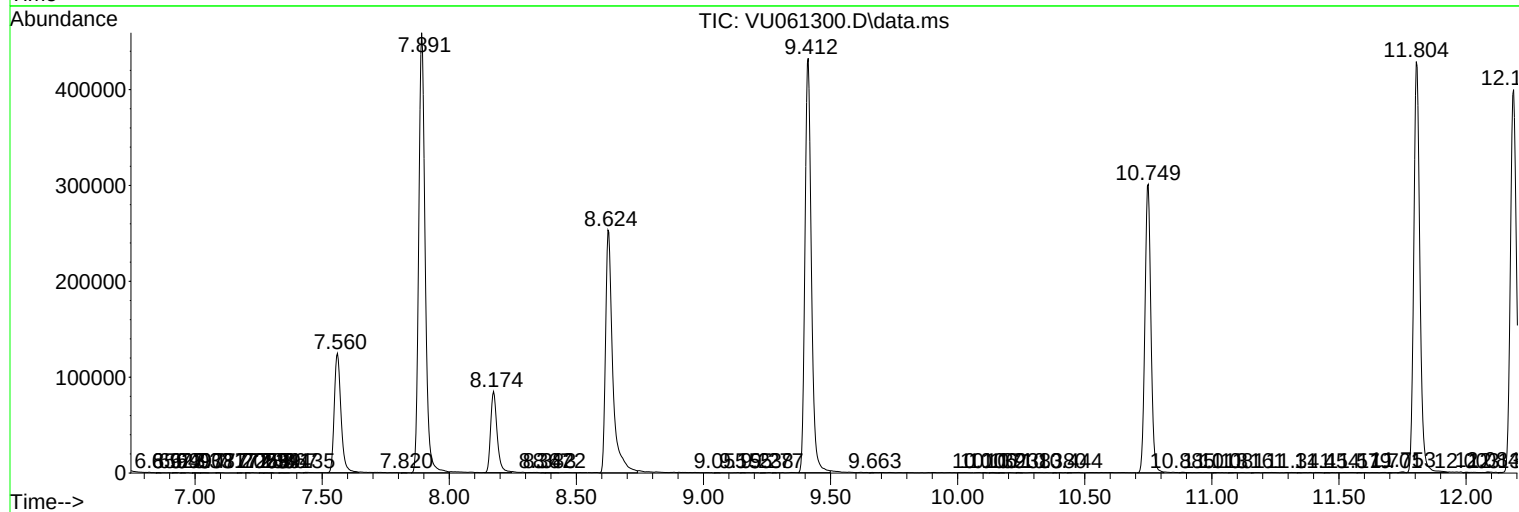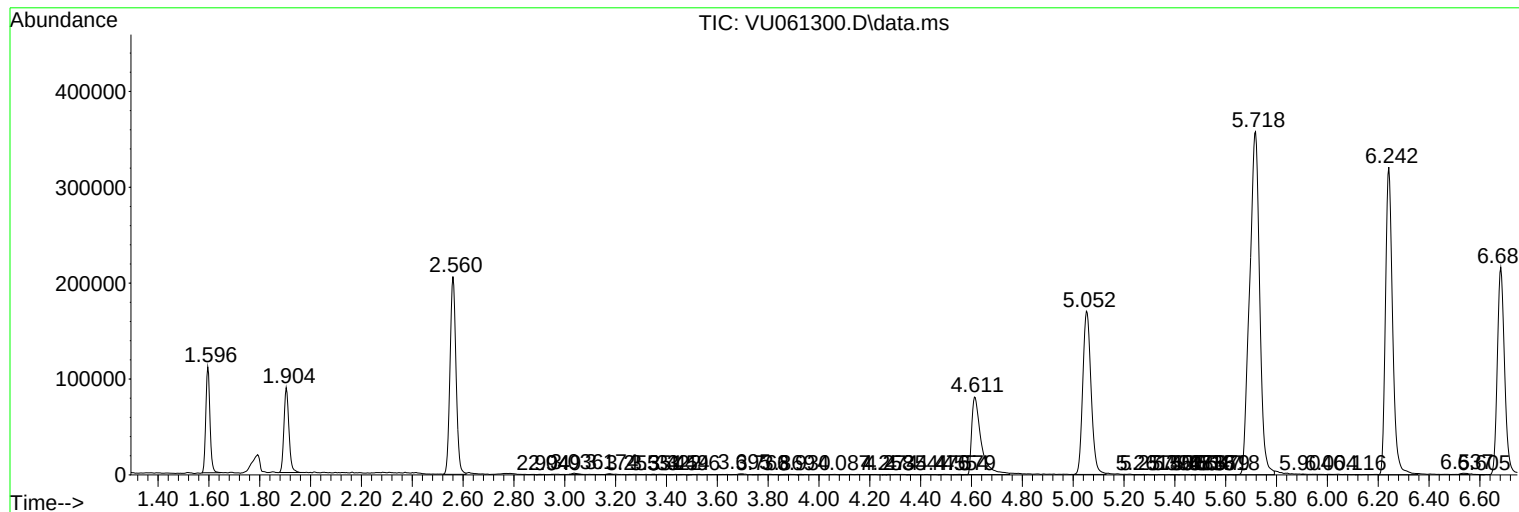

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061300.D
Acq On : 30 Oct 2024 14:19
Operator : MD/SY
Sample : P4582-07
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061300.D
Acq On : 30 Oct 2024 14:19
Operator : MD/SY
Sample : P4582-07
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc