


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103024\
Data File : VU061292.D
Acq On : 30 Oct 2024 08:57
Operator : MD/SY
Sample : BFB079
Misc : 5mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB079

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102824WMA.M
Title : VOC Analysis
Last Update : Thu Oct 31 22:49:53 2024

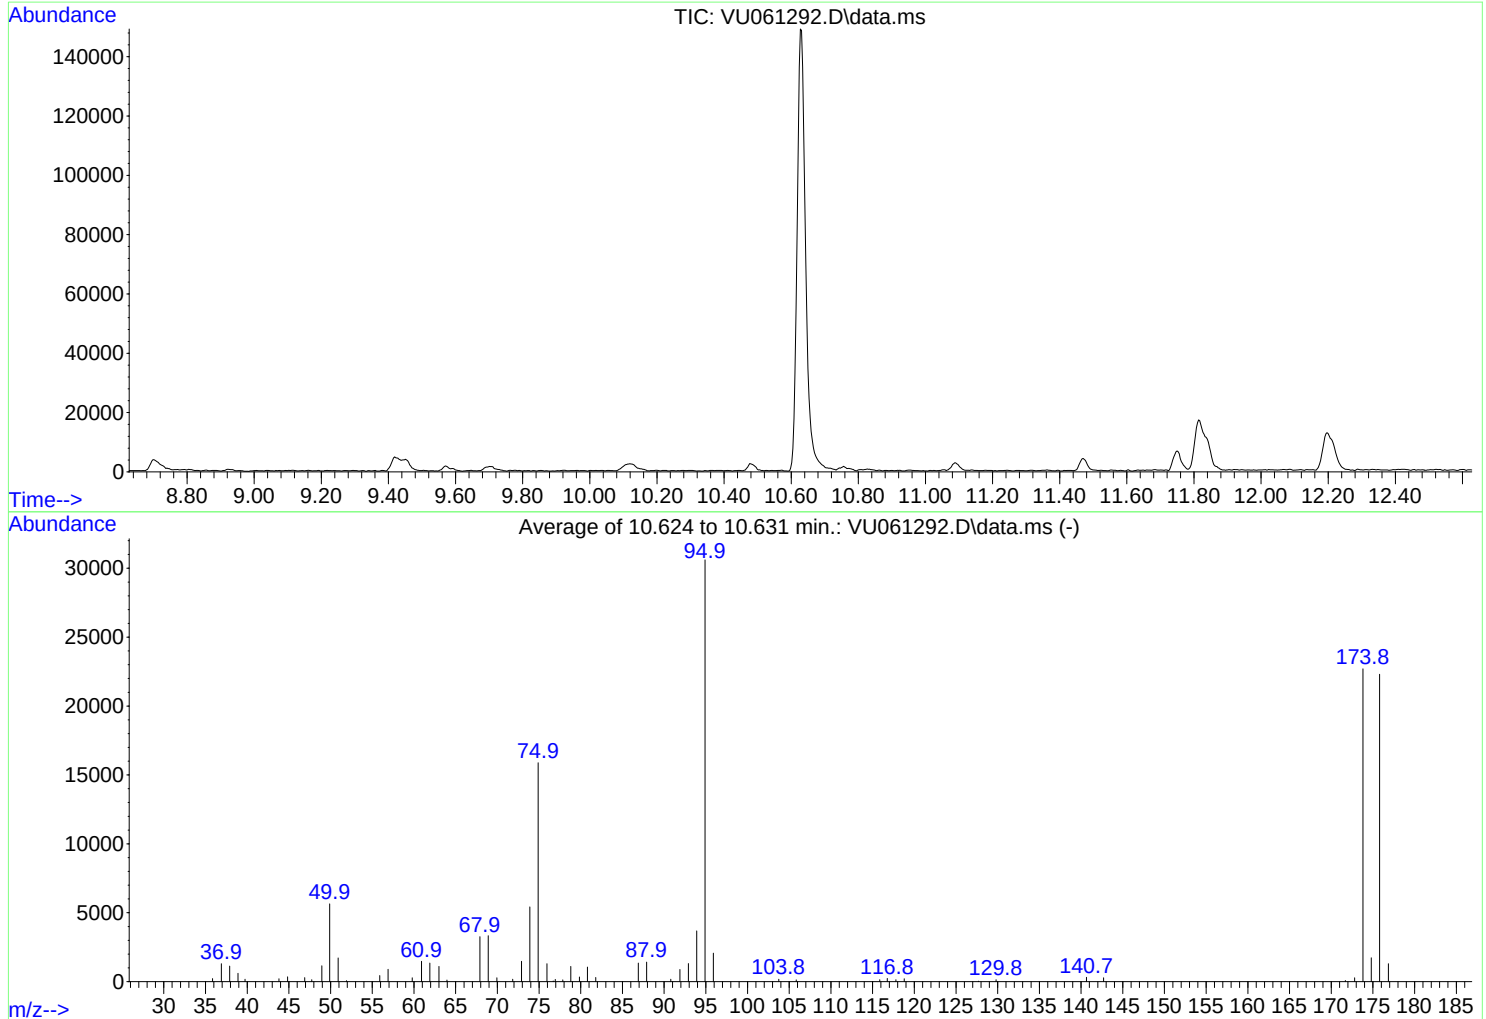

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	5646	PASS
75	95	30	80	51.9	15887	PASS
95	95	100	100	100.0	30611	PASS
96	95	5	9	6.7	2065	PASS
173	174	0.00	2	1.2	283	PASS
174	95	50	120	74.2	22701	PASS
175	174	5	9	7.6	1735	PASS
176	174	95	101	98.3	22307	PASS
177	176	5	9	5.9	1306	PASS

m/z	Abundance
43.80	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	226.0
36.90	1278.0
37.90	1036.0
38.90	529.0
39.70	203.0
43.90	491.0
44.90	313.0
46.90	339.0
47.80	106.0
48.90	1117.0
49.90	5327.0
50.90	1681.0
51.90	111.0
55.90	496.0
56.90	810.0
59.80	260.0
60.90	1400.0
61.90	1261.0
63.00	1017.0
63.90	121.0
67.90	2929.0
68.90	3165.0
69.90	282.0
71.90	186.0
72.90	1392.0
73.90	5374.0
74.90	14851.0
76.00	1279.0
76.70	142.0
77.10	115.0
77.90	128.0
78.80	1029.0
79.80	293.0
80.80	1014.0
81.80	290.0
86.90	1280.0
87.90	1337.0
90.80	152.0
91.90	901.0
92.90	1299.0
93.90	3426.0
94.90	29152.0
95.90	1941.0
103.80	145.0
105.90	103.0
115.90	122.0
116.80	189.0
117.80	126.0
118.80	183.0
129.80	138.0
140.70	279.0
142.70	234.0
172.80	263.0
173.80	20800.0
174.80	1619.0
175.80	20920.0
176.90	1253.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	219.0
36.90	1358.0
37.90	1157.0
38.90	637.0
39.80	165.0
43.80	469.0
44.90	348.0
46.90	264.0
47.70	144.0
48.90	1172.0
49.90	5828.0
50.90	1788.0
51.90	104.0
55.90	456.0
56.90	932.0
59.80	273.0
60.90	1531.0
61.90	1388.0
63.00	1121.0
64.00	124.0
67.90	3362.0
68.90	3432.0
70.00	300.0
71.90	190.0
72.90	1515.0
73.90	5583.0
74.90	16354.0
76.00	1332.0
76.90	169.0
77.90	126.0
78.80	1125.0
79.80	338.0
80.80	1095.0
81.80	314.0
86.90	1369.0
87.90	1500.0
90.80	186.0
91.90	893.0
92.90	1331.0
93.90	3861.0
94.90	31616.0
95.90	2124.0
103.80	190.0
105.90	117.0
115.90	153.0
116.70	235.0
117.80	145.0
118.80	213.0
129.80	154.0
140.60	337.0
142.70	280.0
171.70	109.0
172.80	293.0
173.80	23408.0
174.80	1785.0
175.80	22968.0
176.80	1331.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079

m/z	Abundance
35.90	225.0
36.90	1270.0
37.90	1172.0
38.90	633.0
39.80	147.0
43.90	461.0
44.80	368.0
46.90	258.0
47.80	152.0
49.00	1159.0
49.90	5784.0
50.90	1676.0
55.90	383.0
56.90	956.0
59.80	294.0
60.90	1492.0
61.90	1411.0
63.00	1190.0
64.00	111.0
67.90	3512.0
68.90	3405.0
70.00	261.0
71.80	157.0
72.90	1512.0
73.90	5307.0
74.90	16456.0
75.90	1282.0
76.90	201.0
77.80	116.0
78.80	1142.0
79.90	366.0
80.80	1060.0
81.80	321.0
86.90	1383.0
87.90	1417.0
90.80	176.0
91.90	850.0
92.90	1296.0
93.90	3750.0
94.90	31064.0
95.90	2130.0
103.70	201.0
105.80	150.0
115.80	138.0
116.70	270.0
117.80	158.0
118.80	217.0
127.70	124.0
129.80	135.0
140.60	314.0
142.70	311.0
171.70	151.0
172.80	294.0
173.80	23896.0
174.80	1801.0
175.80	23032.0
176.80	1334.0

Instrument :
MSVOA_U
ClientSampleId :
BFB079