


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU103119\
Data File : VU035555.D
Acq On : 30 Oct 2019 12:26
Operator : JC/SP
Sample : BFB47
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Title : VOC Analysis
Last Update : Thu Nov 07 08:49:29 2019

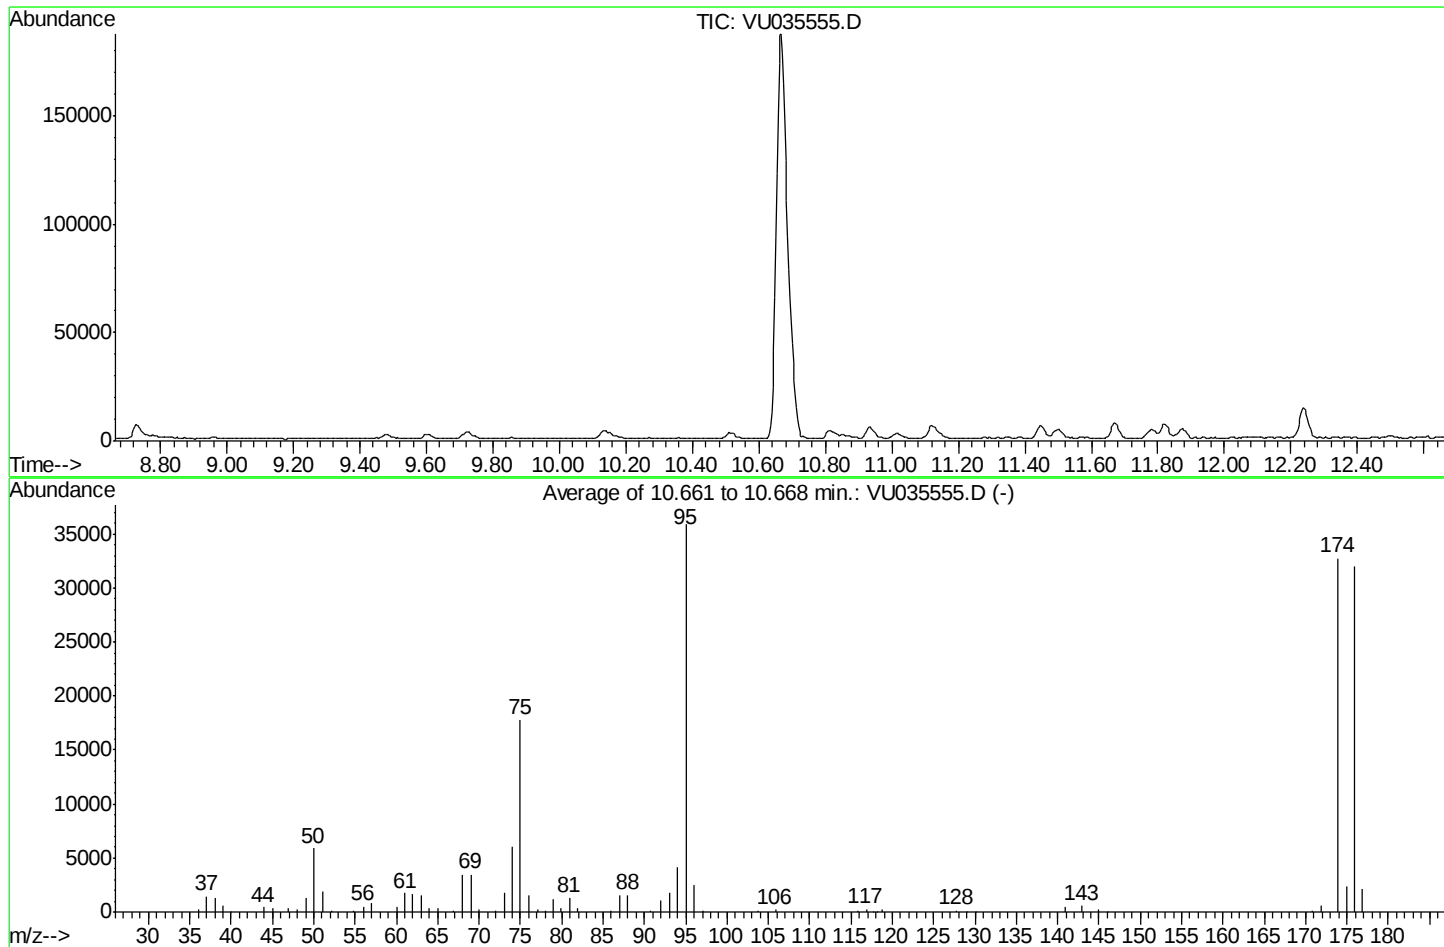

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2887

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	5920	PASS
75	95	30	80	49.6	17821	PASS
95	95	100	100	100.0	35901	PASS
96	95	5	9	6.9	2495	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.2	32744	PASS
175	174	5	9	7.3	2406	PASS
176	174	95	101	97.8	32026	PASS
177	176	5	9	6.6	2115	PASS

m/z	Abundance
36.00	221.0
37.00	1357.0
38.00	1265.0
38.90	557.0
40.00	257.0
44.00	1234.0
45.00	309.0
47.00	428.0
47.90	225.0
49.00	1289.0
50.00	5560.0
51.00	1884.0
54.80	167.0
56.00	450.0
57.00	796.0
60.00	470.0
61.00	1731.0
62.00	1638.0
63.00	1515.0
63.90	363.0
64.90	294.0
66.90	105.0
68.00	3375.0
69.00	3229.0
70.00	239.0
71.90	172.0
73.00	1820.0
74.00	5814.0
75.00	17064.0
76.00	1521.0
77.00	239.0
78.10	107.0
78.90	1219.0
79.80	341.0
80.90	1287.0
81.90	269.0
85.90	105.0
86.90	1318.0
88.00	1349.0
90.80	119.0
91.90	1023.0
93.00	1729.0
94.00	3847.0
95.00	34592.0
96.00	2526.0
97.00	108.0
103.80	100.0
105.90	193.0
115.80	120.0
116.90	250.0
118.10	106.0
118.80	187.0
127.80	140.0
128.90	111.0
140.90	461.0
143.00	496.0
145.00	319.0
171.90	549.0
173.90	31040.0
174.90	2297.0
175.90	30160.0
176.90	2108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	288.0
37.00	1464.0
38.00	1362.0
39.00	584.0
39.90	260.0
44.00	1345.0
45.00	376.0
47.00	410.0
47.90	221.0
49.00	1429.0
50.00	5959.0
51.00	1957.0
52.10	102.0
54.90	186.0
56.00	487.0
57.00	832.0
60.00	477.0
61.00	1758.0
62.00	1734.0
63.00	1605.0
63.90	356.0
65.00	388.0
66.90	123.0
68.00	3498.0
69.00	3564.0
70.00	297.0
71.90	193.0
73.00	1869.0
74.00	6232.0
75.00	18096.0
76.00	1519.0
77.00	235.0
78.00	139.0
78.90	1267.0
79.90	327.0
80.90	1382.0
81.90	345.0
85.90	105.0
87.00	1575.0
87.90	1594.0
90.80	127.0
92.00	1075.0
93.00	1835.0
94.00	4353.0
95.00	36600.0
96.00	2580.0
97.00	128.0
103.80	134.0
105.80	237.0
115.80	128.0
116.80	276.0
118.80	239.0
127.80	164.0
130.00	111.0
140.90	437.0
142.90	573.0
145.00	300.0
170.80	128.0
171.90	580.0
173.90	33552.0
174.90	2453.0
175.90	32784.0
176.90	2193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	333.0
37.00	1486.0
38.00	1344.0
39.00	604.0
39.90	282.0
44.00	1440.0
45.00	360.0
46.90	350.0
48.00	191.0
49.00	1359.0
50.00	6242.0
51.10	1842.0
52.10	116.0
54.90	164.0
56.00	543.0
57.00	888.0
60.00	411.0
61.00	1743.0
62.00	1760.0
63.00	1662.0
64.00	299.0
65.00	455.0
68.00	3490.0
69.00	3655.0
70.00	296.0
72.00	178.0
73.00	1756.0
74.00	6266.0
75.00	18304.0
76.10	1538.0
77.10	223.0
77.90	172.0
78.90	1246.0
79.90	440.0
80.90	1359.0
81.90	393.0
86.90	1698.0
87.90	1762.0
90.80	138.0
92.00	1115.0
93.00	1756.0
94.00	4378.0
95.00	36512.0
96.00	2381.0
97.00	120.0
103.80	160.0
105.80	251.0
115.90	114.0
116.80	256.0
117.70	137.0
118.80	263.0
127.80	126.0
140.90	381.0
142.90	560.0
144.90	275.0
146.00	139.0
170.70	139.0
171.90	610.0
173.90	33640.0
175.00	2468.0
175.90	33136.0
176.90	2046.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

Scan 2887 (10.623 min): VU035555.D
BFB47

m/z	Abundance
40.00	227.0
43.90	903.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47