

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103122\
 Data File : VU051606.D
 Acq On : 31 Oct 2022 12:24
 Operator : JC/MD
 Sample : VU1031WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK123

Quant Time: Nov 01 01:26:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 01 01:25:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	174588	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	187126	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	74570	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	59184	4.501	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.000%	
7) Chloroethane-d5	1.909	69	65568	4.781	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.600%	
11) 1,1-Dichloroethene-d2	2.565	65	22176	4.647	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	93.000%	
20) 2-Butanone-d5	4.623	46	265198	55.690	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	111.380%	
24) Chloroform-d	5.060	84	154459	5.020	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.400%	
26) 1,2-Dichloroethane-d4	5.700	65	89228	5.368	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.400%	
32) Benzene-d6	5.726	84	266668	4.516	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	6.687	67	101498	4.915	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.400%	
41) Toluene-d8	7.896	98	176913	3.810	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.200%	
43) trans-1,3-Dichloroprop...	8.179	79	27890	4.417	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	88.400%	
46) 2-Hexanone-d5	8.632	63	186389	49.040	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	98.080%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	99448	5.256	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	105.200%	
66) 1,2-Dichlorobenzene-d4	12.192	152	68889	5.033	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.600%	
Target Compounds						
					Qvalue	
13) Acetone	2.633	43	9494	3.929	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103122\
Data File : VU051606.D
Acq On : 31 Oct 2022 12:24
Operator : JC/MD
Sample : VU1031WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK123

Quant Time: Nov 01 01:26:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 01 01:25:31 2022
Response via : Initial Calibration

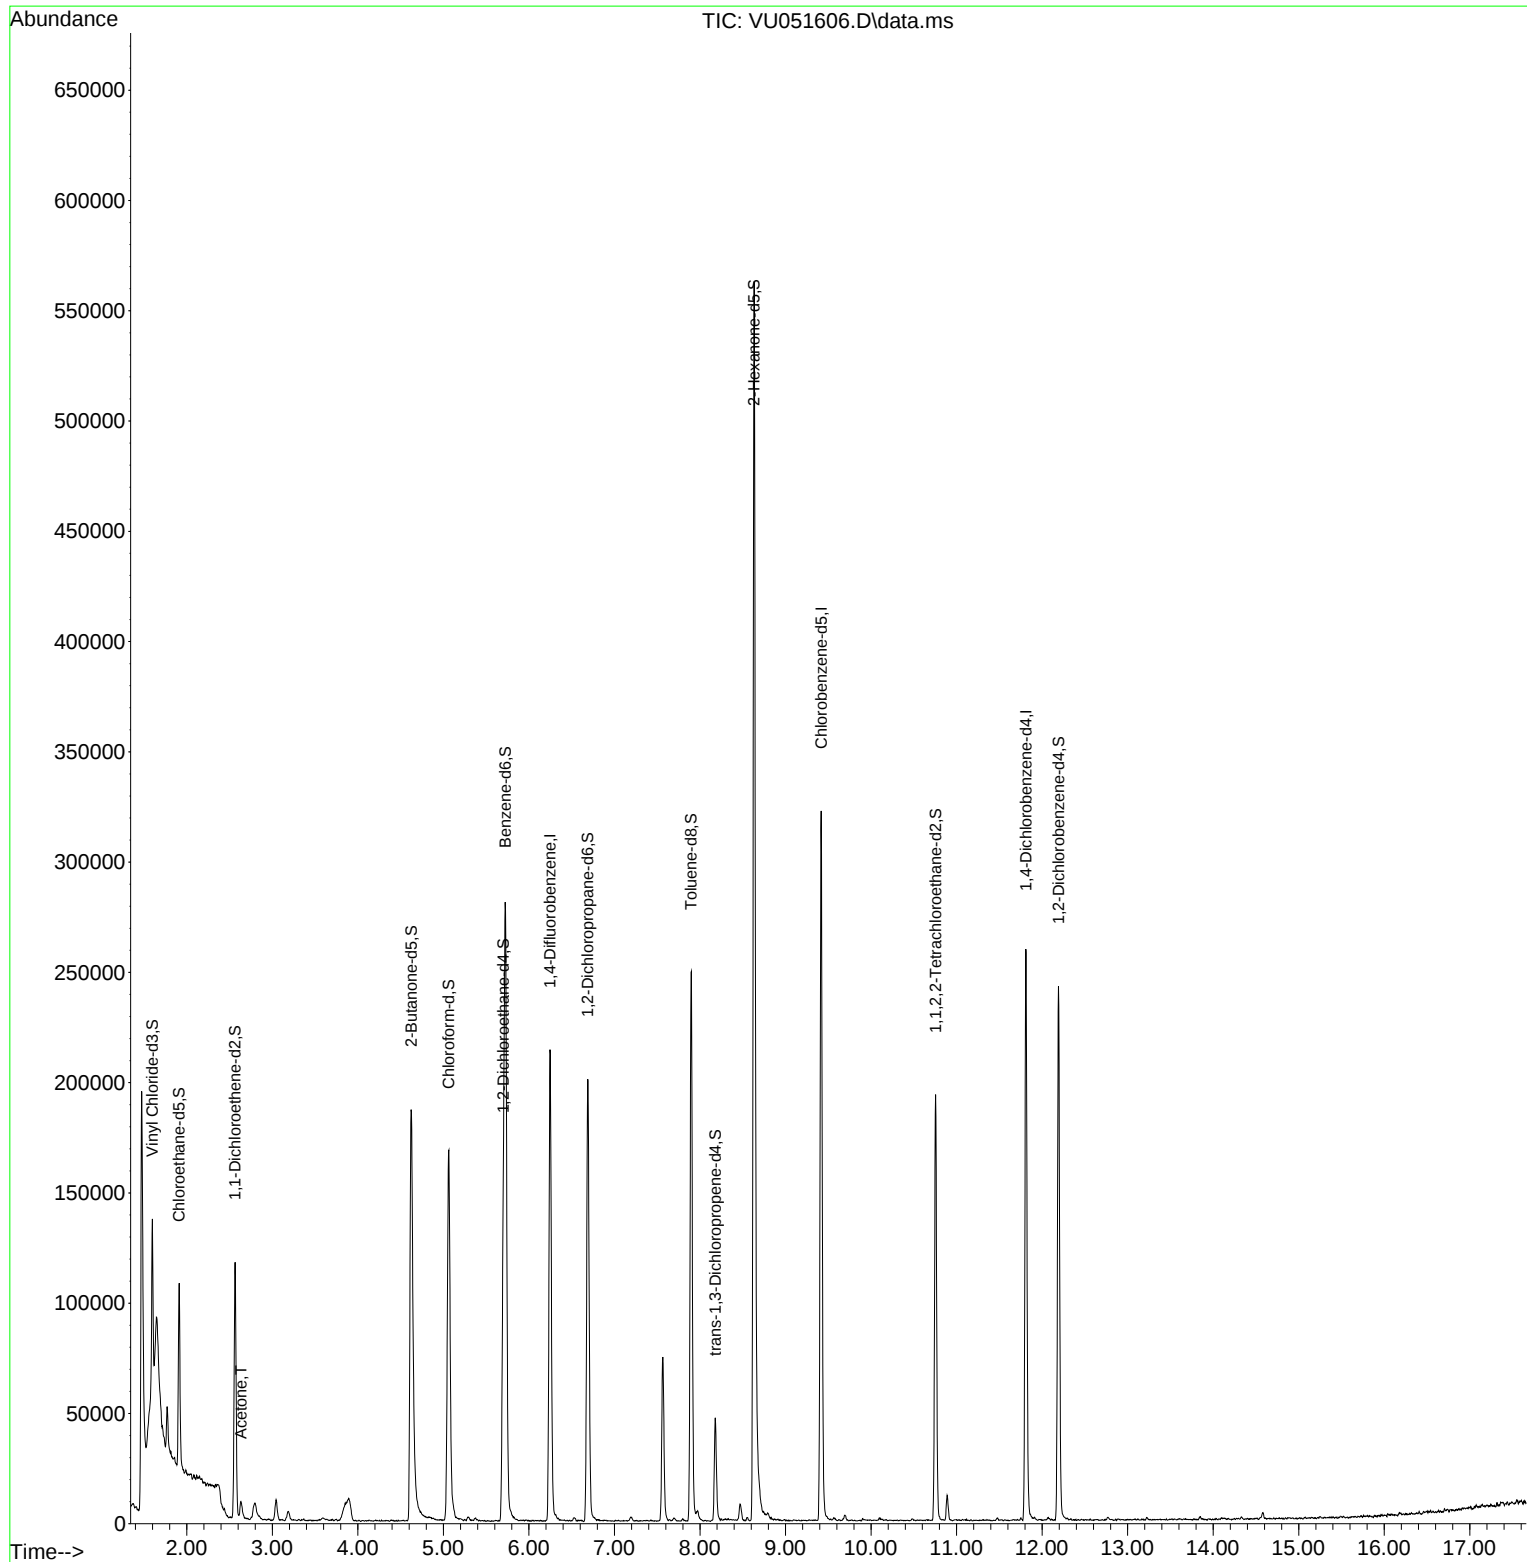

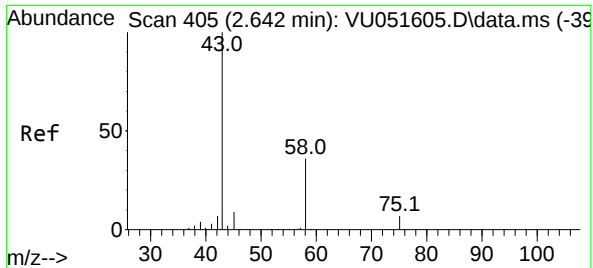

#13
 Acetone
 Concen: 3.929 ug/L
 RT: 2.633 min Scan# 40
 Delta R.T. -0.009 min
 Lab File: VU051606.D
 Acq: 31 Oct 2022 12:24

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK123

Tgt Ion: 43 Resp: 9494
 Ion Ratio Lower Upper
 43 100
 58 36.0 0.0 73.8

