

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103122\
 Data File : VU051627.D
 Acq On : 31 Oct 2022 22:08
 Operator : JC/MD
 Sample : VU1031WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK124

Quant Time: Nov 01 02:35:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 01 02:34:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	178563	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	188982	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	73254	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	51086	3.799	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.000%
7) Chloroethane-d5	1.909	69	63258	4.510	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.562	65	19652	4.026	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.600%
20) 2-Butanone-d5	4.617	46	276264	56.722	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.440%
24) Chloroform-d	5.060	84	147017	4.672	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	5.700	65	87244	5.132	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.600%
32) Benzene-d6	5.726	84	251239	4.213	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.200%
36) 1,2-Dichloropropane-d6	6.690	67	97706	4.685	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.800%
41) Toluene-d8	7.896	98	169278	3.609	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.200%
43) trans-1,3-Dichloroprop...	8.179	79	25577	4.011	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.200%
46) 2-Hexanone-d5	8.632	63	191949	50.007	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.020%
56) 1,1,2,2-Tetrachloroeth...	10.755	84	96615	5.056	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.200%
66) 1,2-Dichlorobenzene-d4	12.192	152	64231	4.777	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds						Qvalue
13) Acetone	2.626	43	12009	4.860	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103122\
Data File : VU051627.D
Acq On : 31 Oct 2022 22:08
Operator : JC/MD
Sample : VU1031WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK124

Quant Time: Nov 01 02:35:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 01 02:34:58 2022
Response via : Initial Calibration

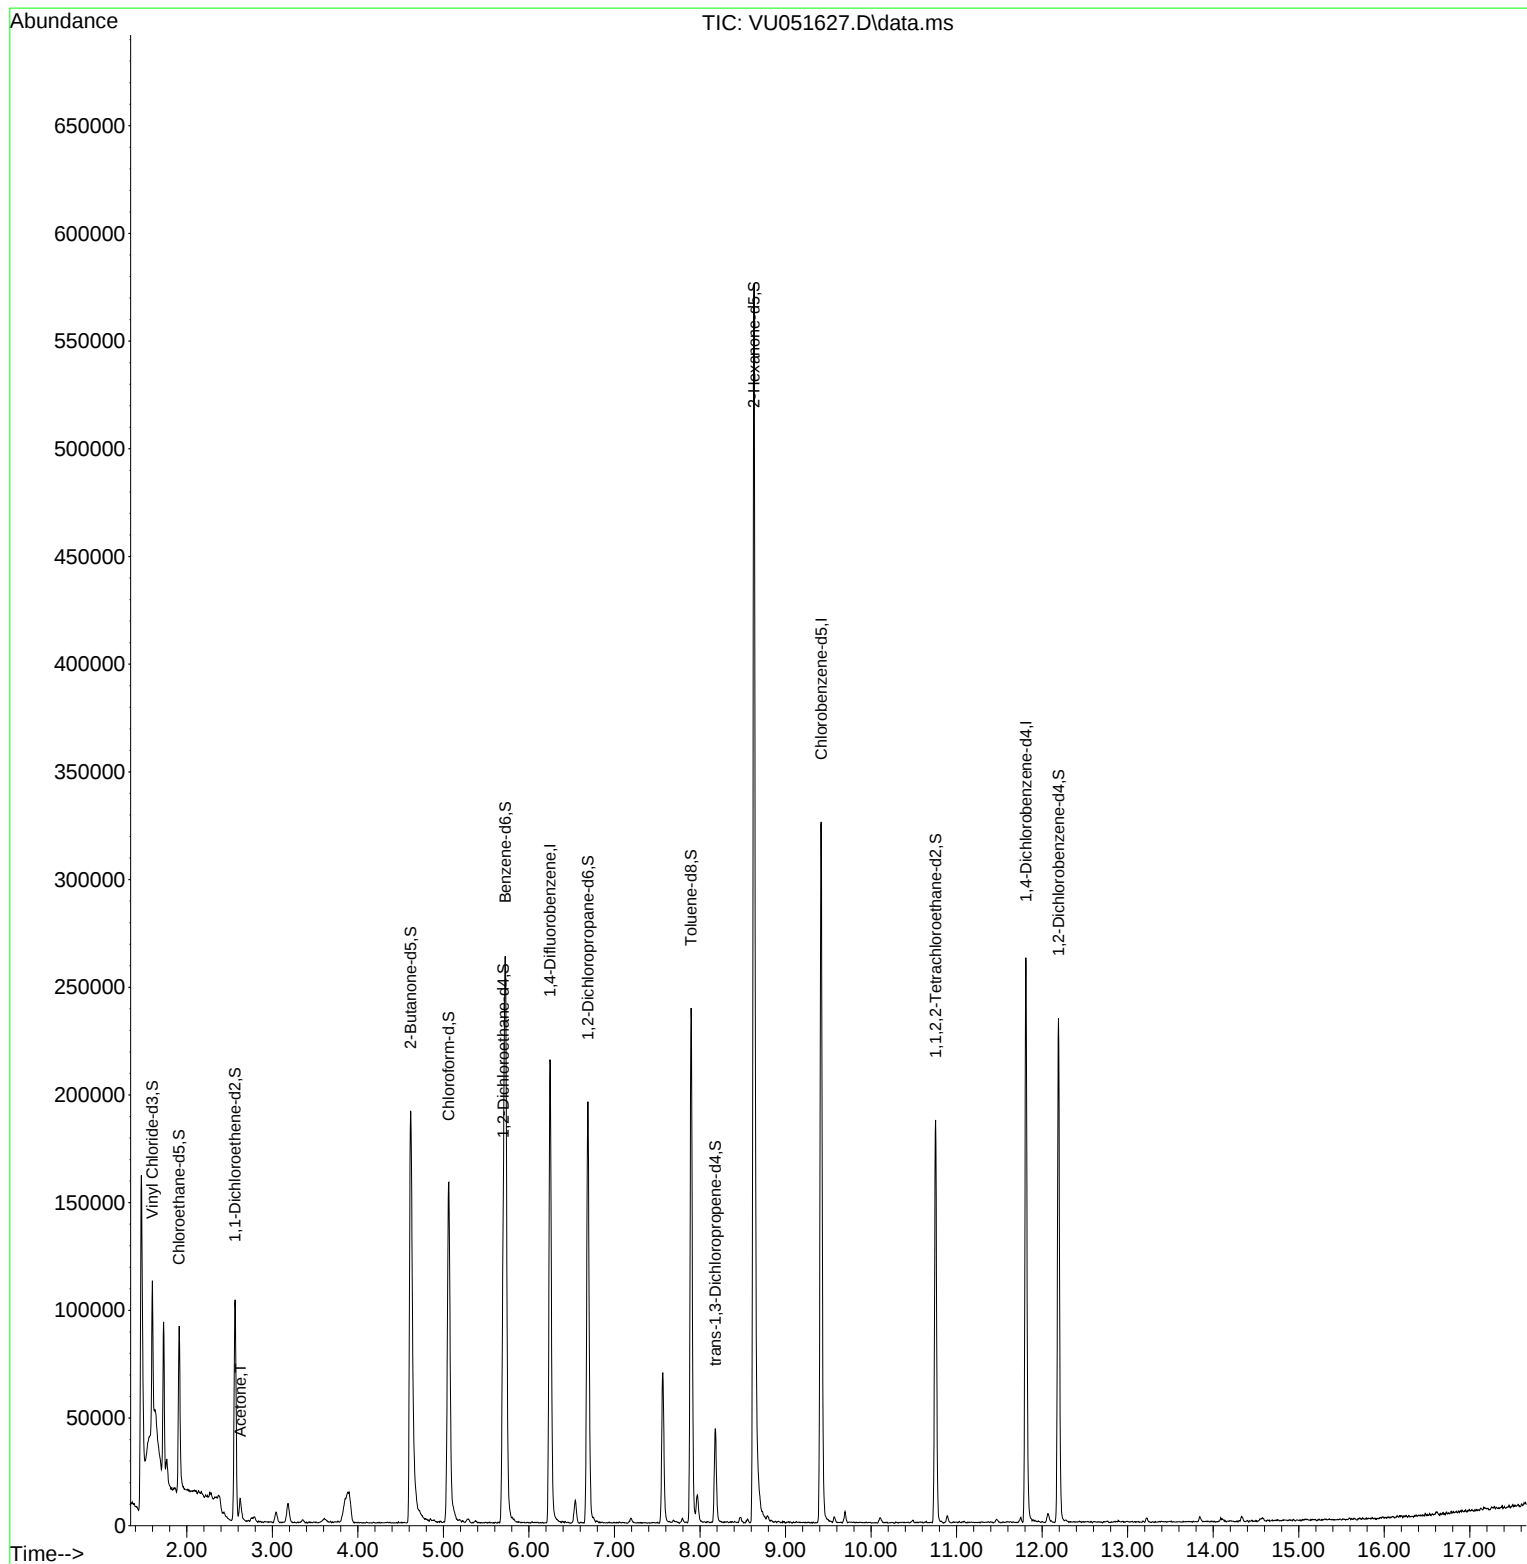

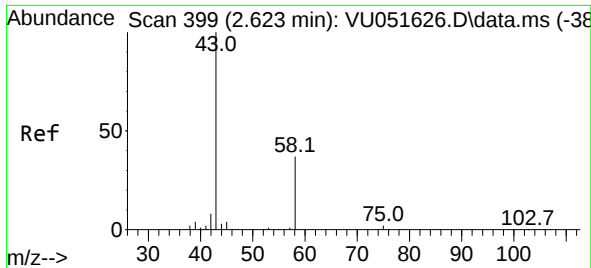

#13
 Acetone
 Concen: 4.860 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051627.D
 Acq: 31 Oct 2022 22:08

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK124

Tgt Ion: 43 Resp: 12009
 Ion Ratio Lower Upper
 43 100
 58 35.8 0.0 73.8

