

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
 Data File : VU056014.D
 Acq On : 31 Oct 2023 15:09
 Operator : MD/SY
 Sample : VIBLK150
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK150

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	113	rVB	110222	130322	12.47%	1.461%
2	1.914	186	194	211	rVB	97694	138153	13.22%	1.549%
3	2.566	385	397	418	rBV	196759	323769	30.99%	3.631%
4	3.046	536	546	564	rVB3	11495	23477	2.25%	0.263%
5	4.637	1029	1041	1083	rBV	110197	392637	37.58%	4.403%
6	5.062	1157	1173	1198	rBV2	206121	474237	45.39%	5.318%
7	5.724	1359	1379	1415	rBV3	391946	1044897	100.00%	11.717%
8	6.248	1528	1542	1565	rBV	379795	756116	72.36%	8.479%
9	6.689	1665	1679	1708	rBV2	247983	499271	47.78%	5.598%
10	7.563	1938	1951	1975	rBV	109916	209506	20.05%	2.349%
11	7.897	2042	2055	2090	rBV	443853	822520	78.72%	9.223%
12	8.180	2131	2143	2164	rBV	66106	122196	11.69%	1.370%
13	8.470	2224	2233	2242	rBV2	6205	10551	1.01%	0.118%
14	8.550	2246	2258	2273	rBV2	112886	199737	19.12%	2.240%
15	8.634	2273	2284	2323	rVV3	450503	1041553	99.68%	11.679%
16	9.415	2515	2527	2552	rBV	517675	937275	89.70%	10.510%
17	10.753	2931	2943	2959	rBV	181829	302698	28.97%	3.394%
18	10.891	2974	2986	2999	rBV2	14767	24240	2.32%	0.272%
19	11.810	3260	3272	3296	rBV	479701	804901	77.03%	9.026%
20	12.190	3376	3390	3416	rBV	384544	659940	63.16%	7.400%




Sum of corrected areas: 8917996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056014.D
Acq On : 31 Oct 2023 15:09
Operator : MD/SY
Sample : VIBLK150
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

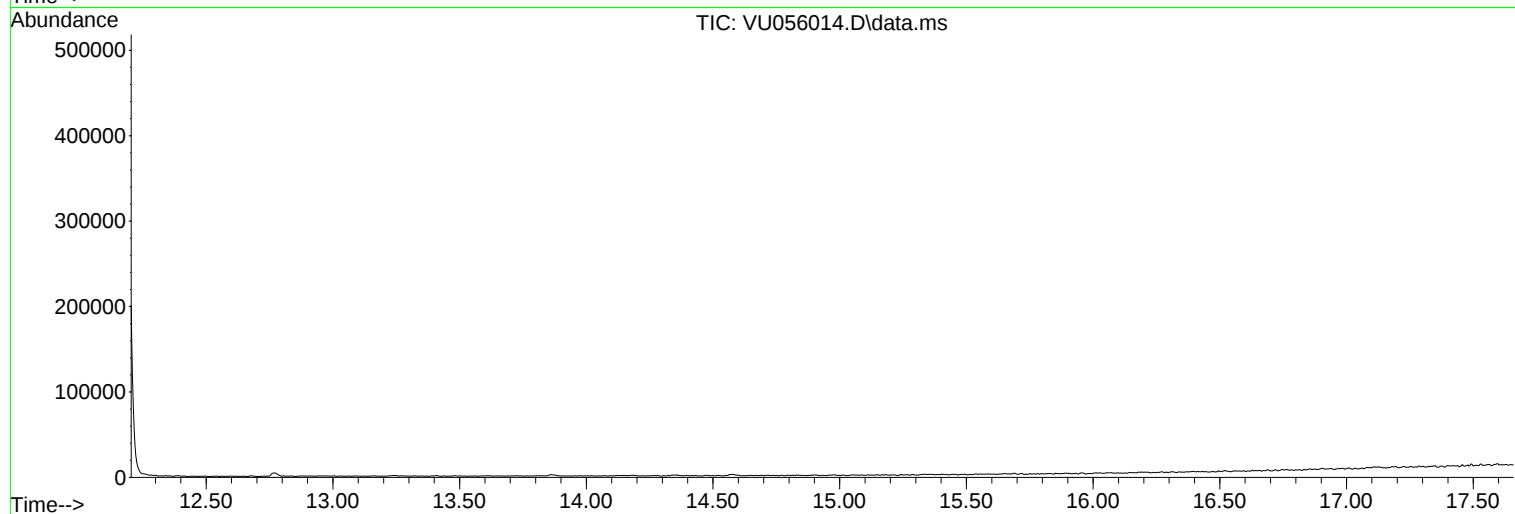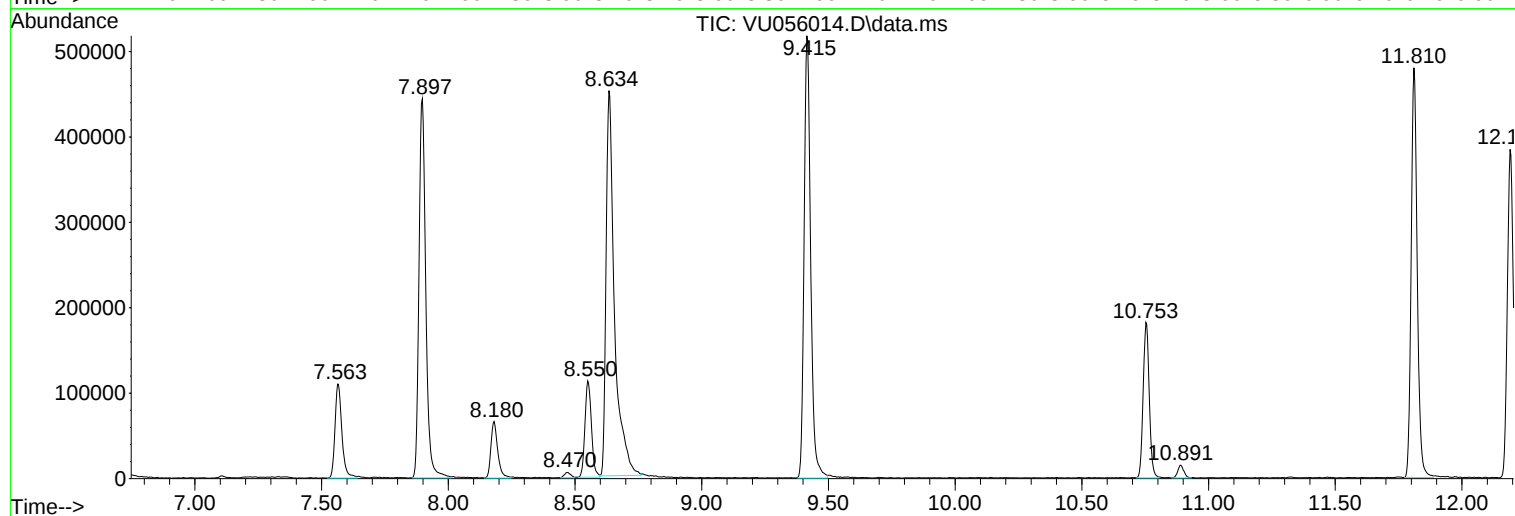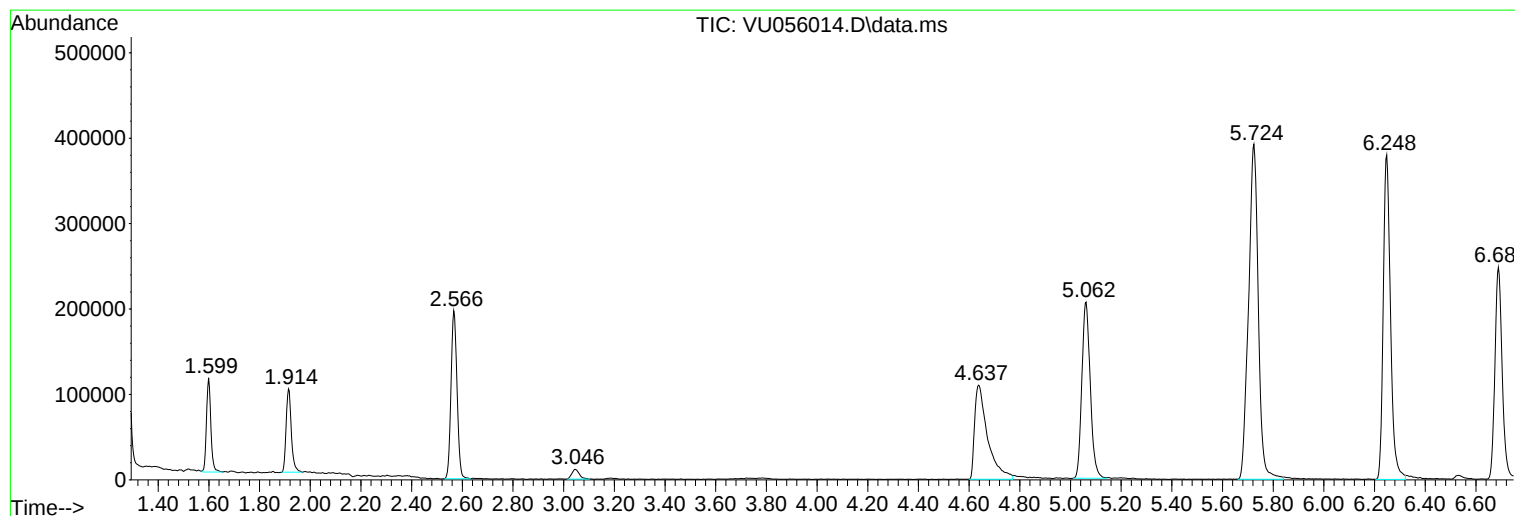

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056014.D
Acq On : 31 Oct 2023 15:09
Operator : MD/SY
Sample : VIBLK150
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056014.D
Acq On : 31 Oct 2023 15:09
Operator : MD/SY
Sample : VIBLK150
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK150

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
