

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
 Data File : VU056015.D
 Acq On : 31 Oct 2023 15:43
 Operator : MD/SY
 Sample : VIBLK151
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK151

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	112	rVB	114526	133298	11.85%	1.418%
2	1.914	186	194	212	rBV	99933	140182	12.46%	1.491%
3	2.567	385	397	412	rBV	198865	326697	29.05%	3.475%
4	3.049	534	547	566	rBV2	13406	27549	2.45%	0.293%
5	3.187	576	590	607	rVB	14682	34247	3.04%	0.364%
6	4.640	1023	1042	1096	rBV2	124497	523803	46.57%	5.571%
7	5.062	1157	1173	1198	rBV	209202	478069	42.51%	5.085%
8	5.724	1358	1379	1409	rBV2	403702	1070677	95.19%	11.387%
9	6.248	1529	1542	1574	rBV	387521	775291	68.93%	8.246%
10	6.689	1665	1679	1699	rBV	250835	506413	45.03%	5.386%
11	7.566	1939	1952	1974	rBV2	115757	217634	19.35%	2.315%
12	7.898	2041	2055	2083	rBV	460804	847680	75.37%	9.016%
13	8.180	2132	2143	2164	rBV	66466	125545	11.16%	1.335%
14	8.553	2246	2259	2273	rBV3	56023	100257	8.91%	1.066%
15	8.637	2273	2285	2331	rVV2	479364	1124723	100.00%	11.962%
16	8.914	2361	2371	2387	rBV5	5938	12046	1.07%	0.128%
17	9.415	2515	2527	2563	rBV	543126	976357	86.81%	10.384%
18	10.753	2929	2943	2969	rBV	191450	317727	28.25%	3.379%
19	10.891	2973	2986	3000	rVV3	9897	16699	1.48%	0.178%
20	11.811	3260	3272	3291	rBV	535808	898903	79.92%	9.560%
21	12.190	3378	3390	3418	rBV	435719	748485	66.55%	7.961%




Sum of corrected areas: 9402282

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056015.D
Acq On : 31 Oct 2023 15:43
Operator : MD/SY
Sample : VIBLK151
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

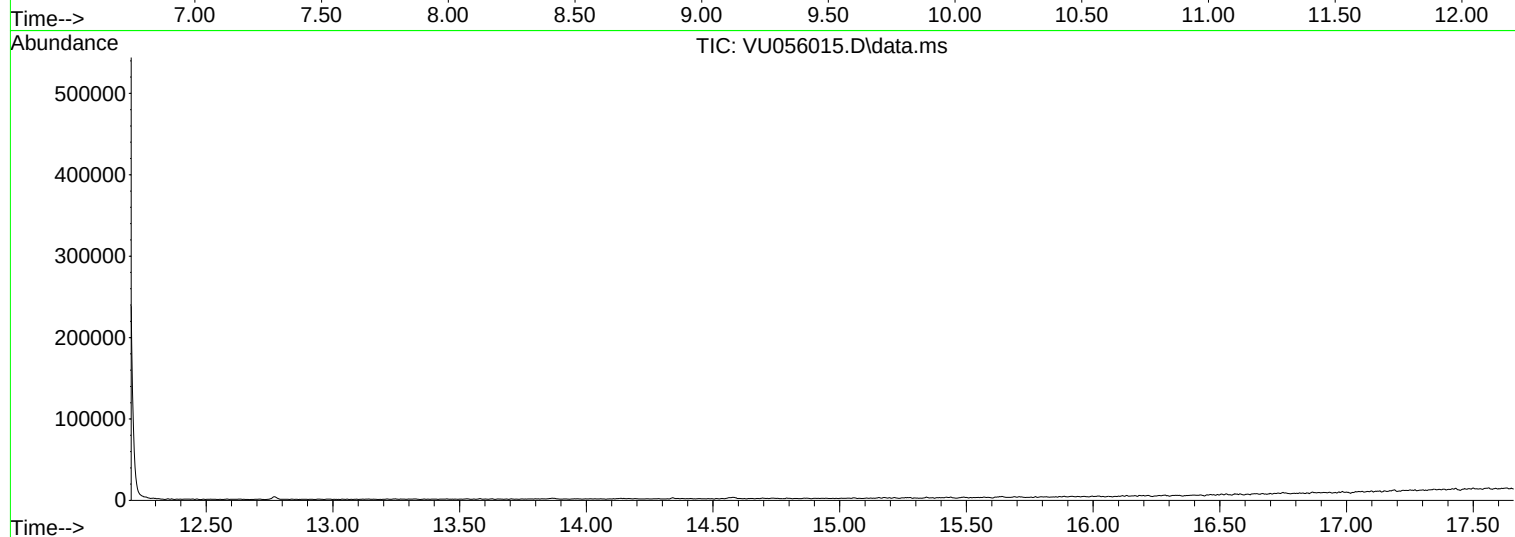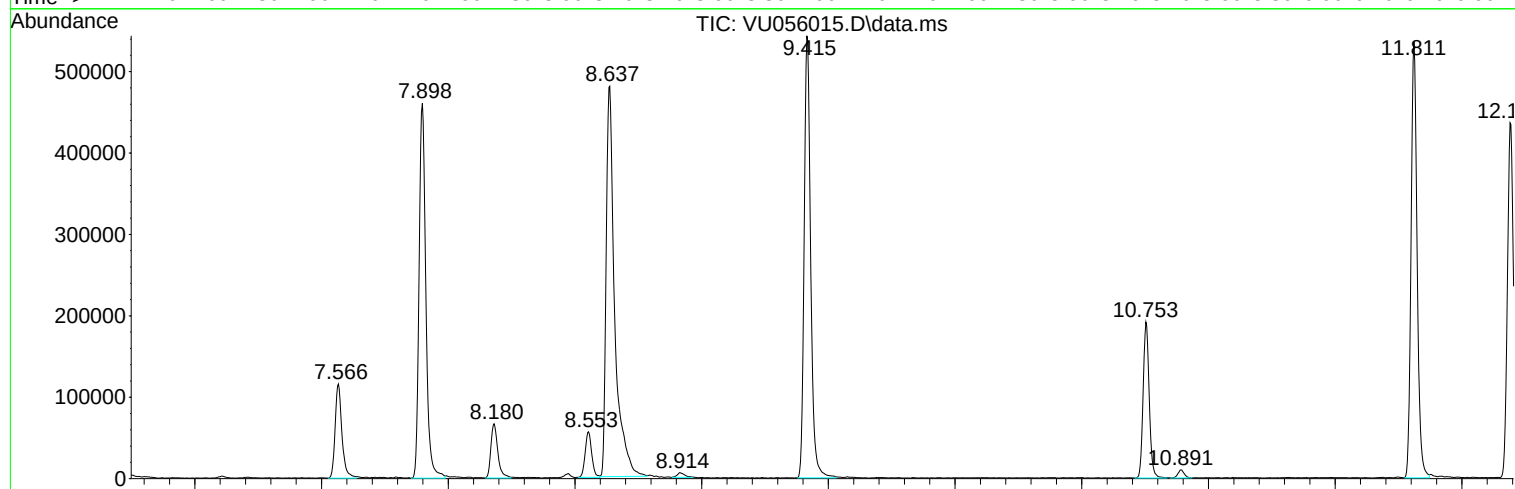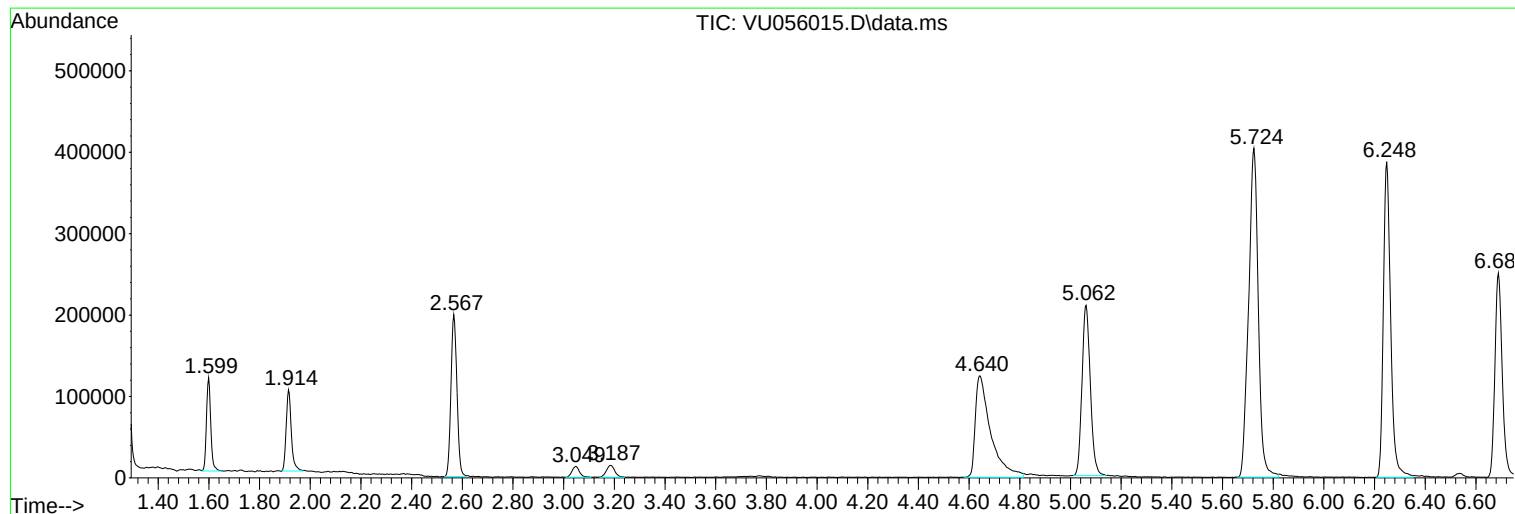

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056015.D
Acq On : 31 Oct 2023 15:43
Operator : MD/SY
Sample : VIBLK151
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056015.D
Acq On : 31 Oct 2023 15:43
Operator : MD/SY
Sample : VIBLK151
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc