

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
 Data File : VU056026.D
 Acq On : 31 Oct 2023 20:33
 Operator : MD/SY
 Sample : 05114-17DL 500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B68DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	84	96	111	rVB2	113719	173680	6.39%	1.482%
2	1.914	186	194	210	rVB	94270	134222	4.94%	1.145%
3	2.567	385	397	414	rBV	188492	314527	11.57%	2.684%
4	3.043	535	545	561	rBV4	19363	38686	1.42%	0.330%
5	3.181	574	588	608	rBV2	34633	81932	3.02%	0.699%
6	4.637	1022	1041	1087	rBV2	133589	487953	17.96%	4.163%
7	5.059	1156	1172	1196	rBV	204216	461387	16.98%	3.937%
8	5.724	1357	1379	1403	rBV2	394626	1044999	38.46%	8.916%
9	6.248	1525	1542	1564	rBV	369309	734883	27.04%	6.270%
10	6.689	1662	1679	1701	rBV	243229	493606	18.16%	4.212%
11	7.563	1938	1951	1972	rBV	108859	204886	7.54%	1.748%
12	7.894	2040	2054	2075	rBV	440216	811058	29.85%	6.920%
13	8.177	2132	2142	2162	rBV2	63066	115882	4.26%	0.989%
14	8.550	2243	2258	2274	rBV	1581487	2717378	100.00%	23.185%
15	8.634	2274	2284	2323	rVV3	509250	1157051	42.58%	9.872%
16	9.415	2514	2527	2559	rBV	519262	915932	33.71%	7.815%
17	10.753	2930	2943	2964	rBV	188790	312735	11.51%	2.668%
18	11.811	3258	3272	3300	rBV	487869	815001	29.99%	6.954%
19	12.190	3378	3390	3413	rBV	414091	704380	25.92%	6.010%




Sum of corrected areas: 11720178

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056026.D
Acq On : 31 Oct 2023 20:33
Operator : MD/SY
Sample : 05114-17DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B68DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

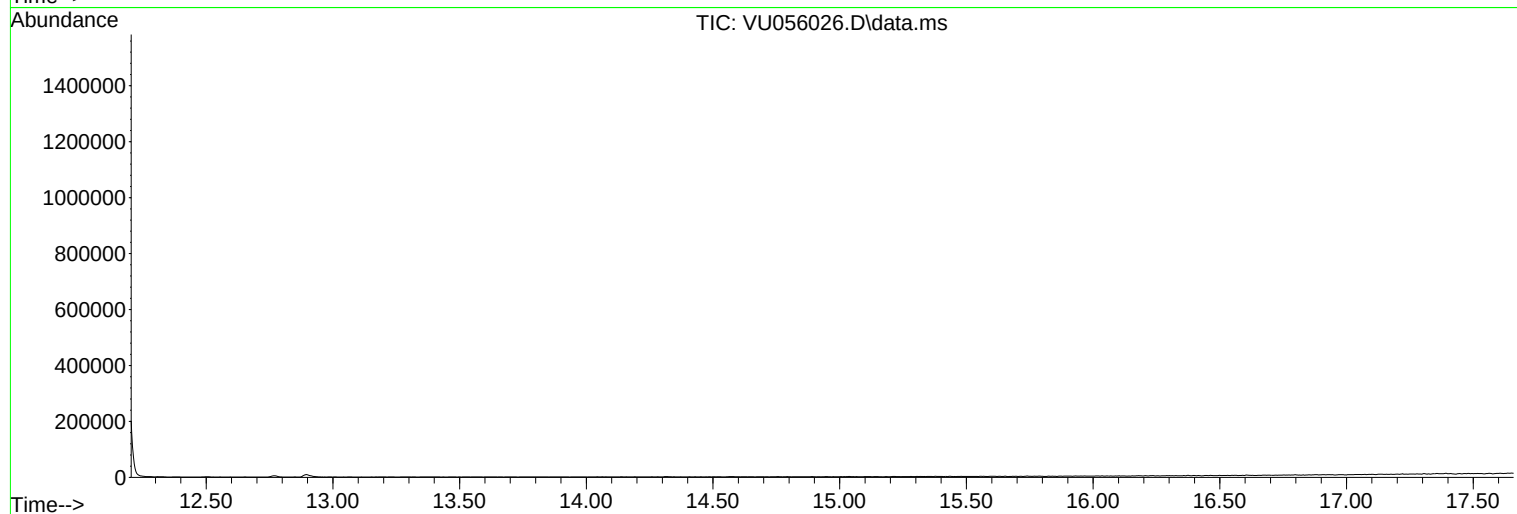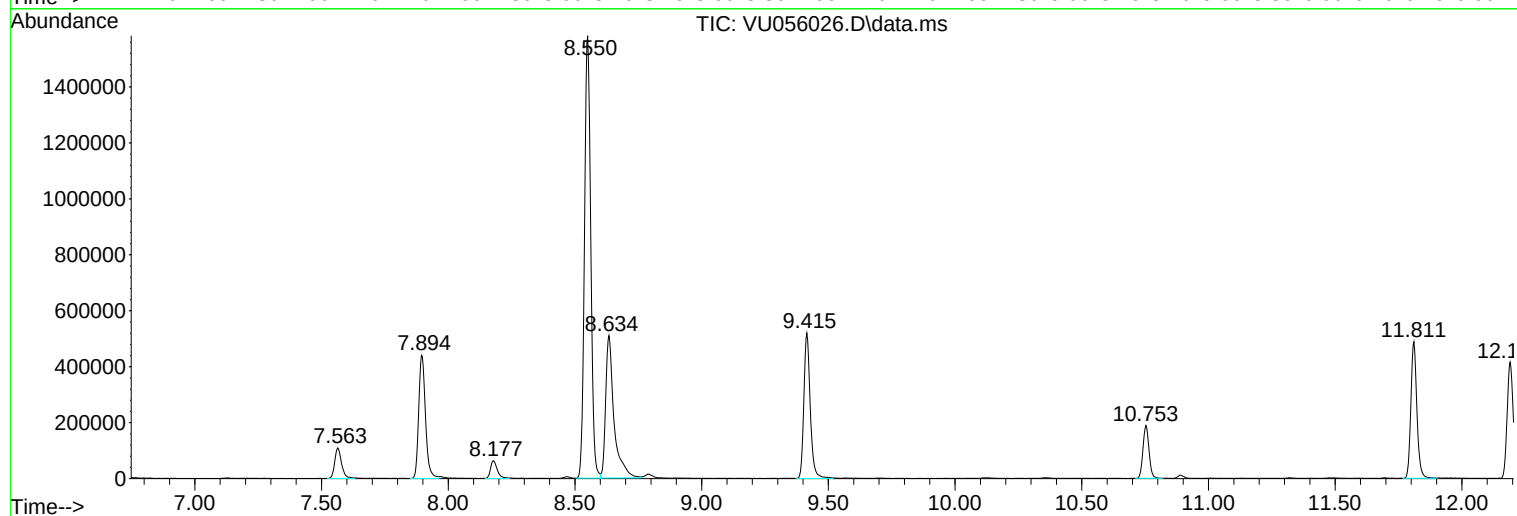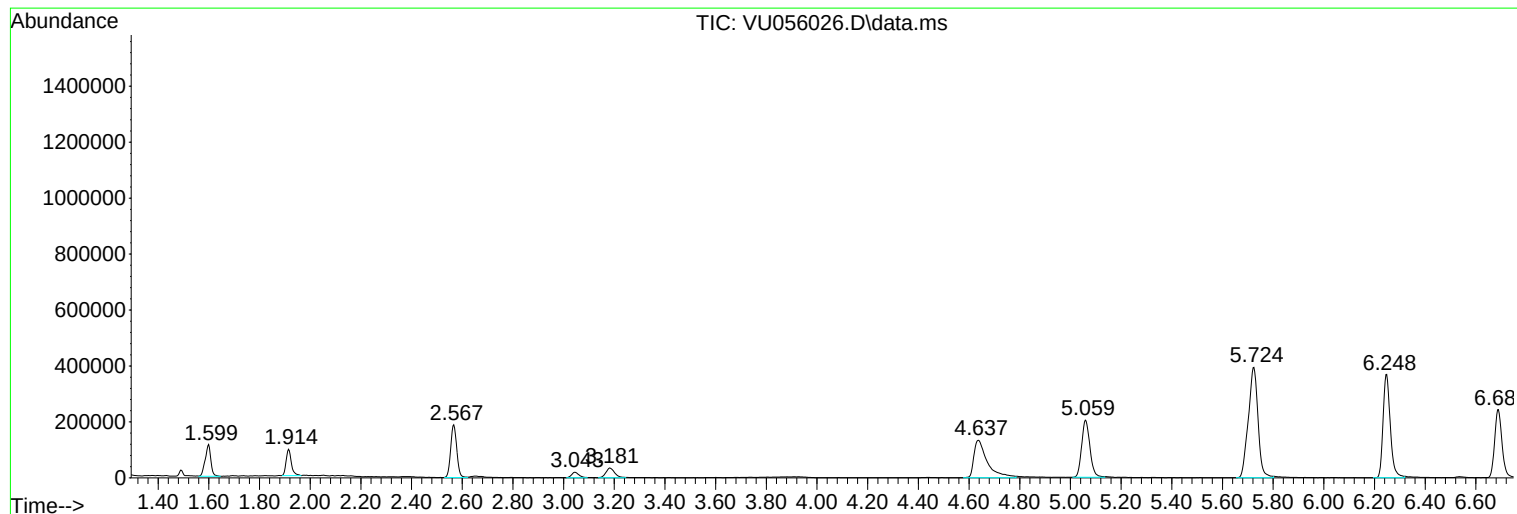

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056026.D
Acq On : 31 Oct 2023 20:33
Operator : MD/SY
Sample : 05114-17DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B68DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103123\
Data File : VU056026.D
Acq On : 31 Oct 2023 20:33
Operator : MD/SY
Sample : 05114-17DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B68DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc