

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
 Data File : VU063662.D
 Acq On : 31 Oct 2025 15:29
 Operator : MD/SY
 Sample : VU1031WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1031WBL01

Quant Time: Nov 03 00:57:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Mon Nov 03 00:51:51 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.081	96	57963	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.611	95	24052	0.917	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	
68) 1,2-Dichlorobenzene-d4	12.171	152	21876	0.931	ug/l	0.00
Spiked Amount 1.000			Recovery	=	93.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063662.D
Acq On : 31 Oct 2025 15:29
Operator : MD/SY
Sample : VU1031WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1031WBL01

Quant Time: Nov 03 00:57:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Mon Nov 03 00:51:51 2025
Response via : Initial Calibration




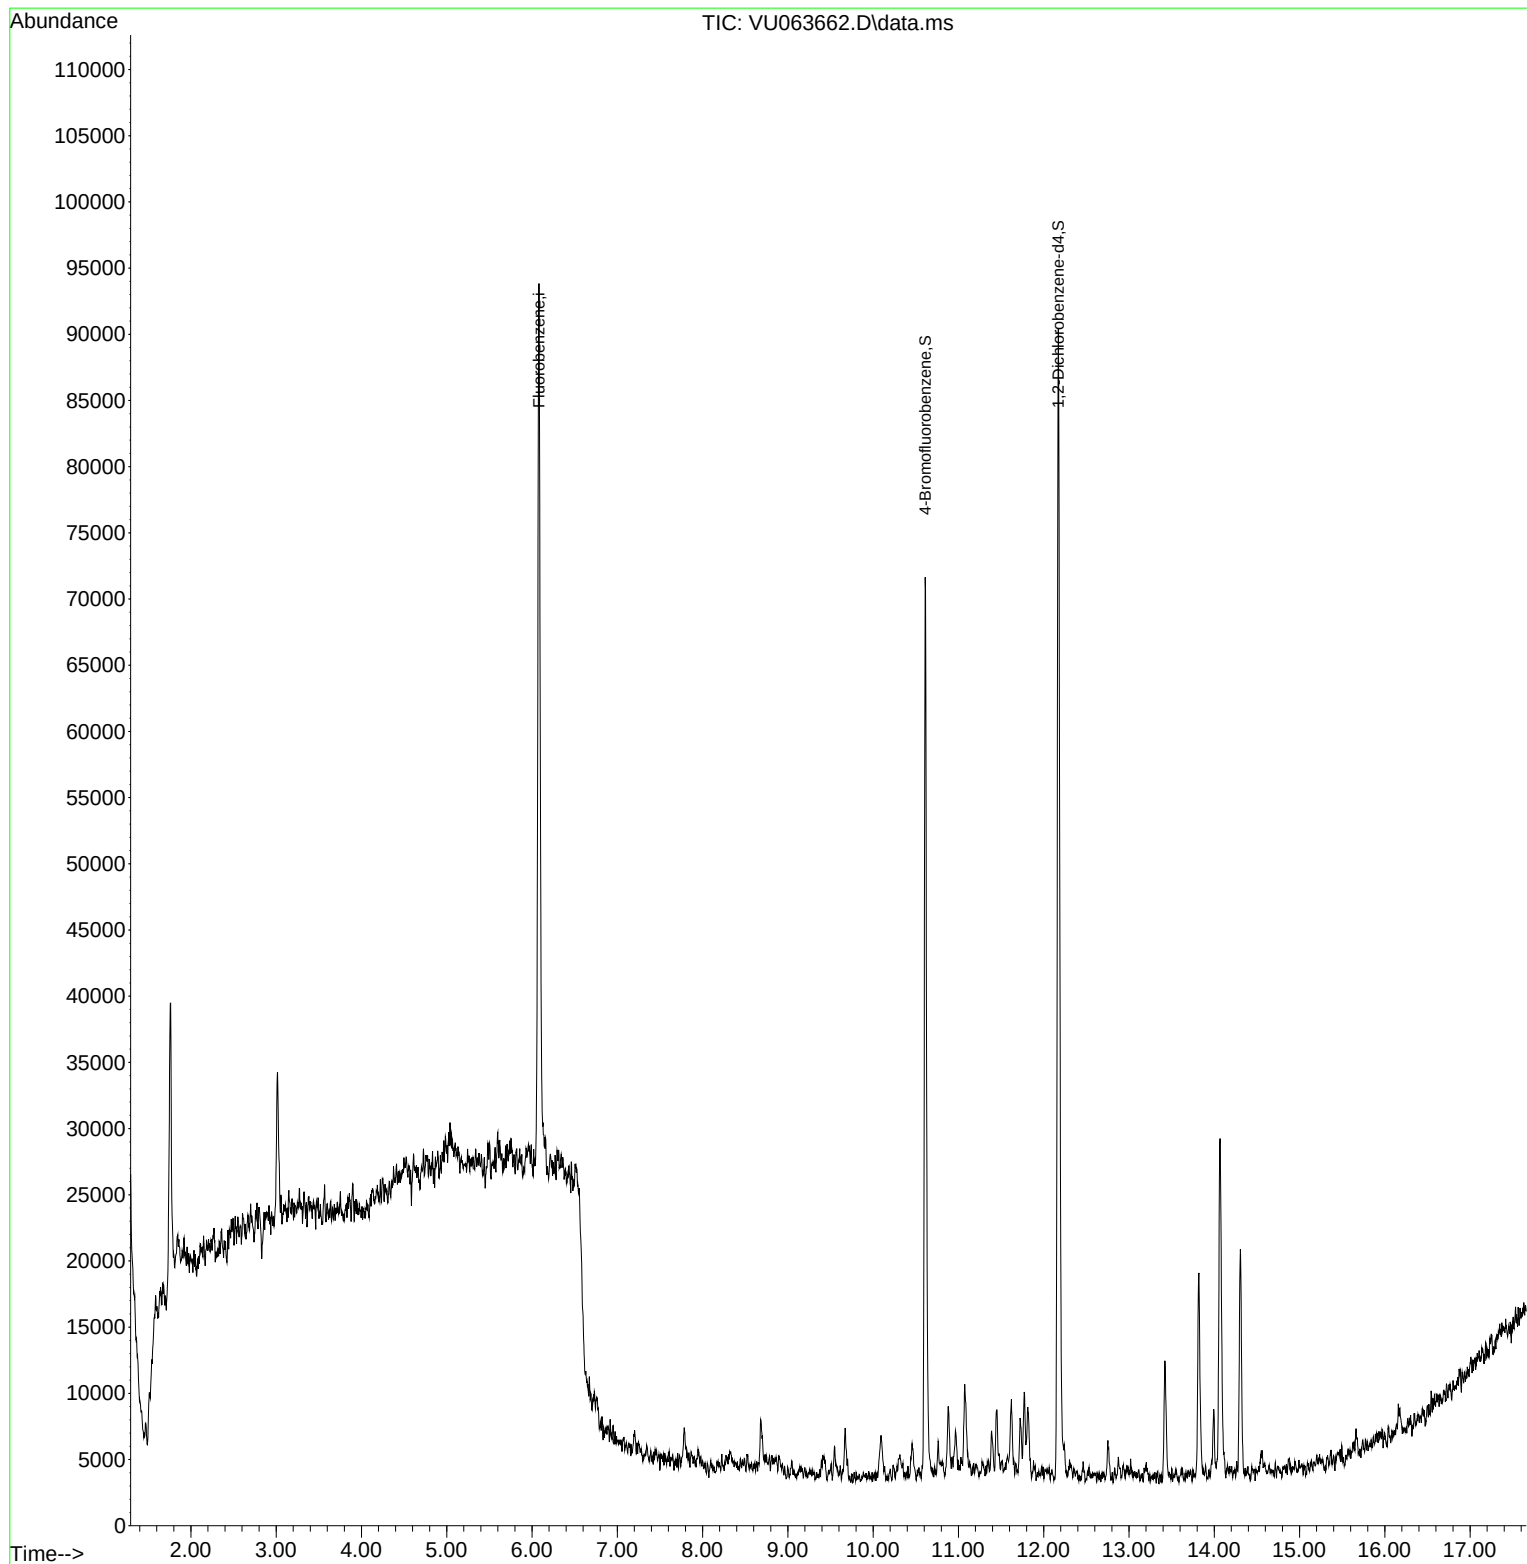


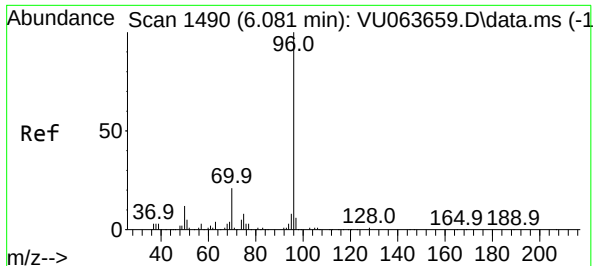

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.081 min Scan# 1490
Delta R.T. -0.000 min
Lab File: VU063662.D
Acq: 31 Oct 2025 15:29




Instrument :
MSVOA_U
ClientSampleId :
VU1031WBL01


Tgt Ion:	96	Resp:	57963
Ion Ratio	Lower	Upper	
96	100		
70	19.7	15.3	22.9
95	8.5	6.5	9.7
97	6.0	0.0	0.0

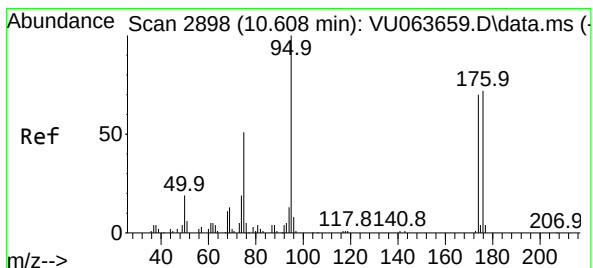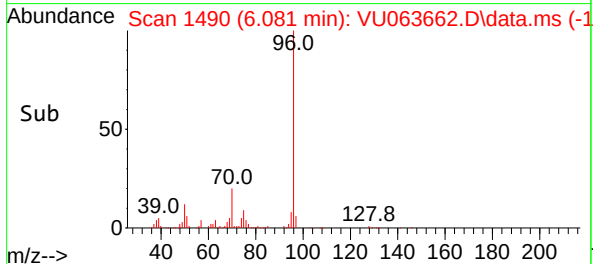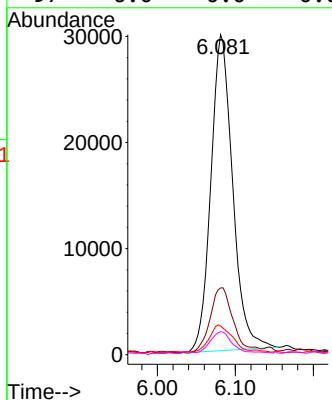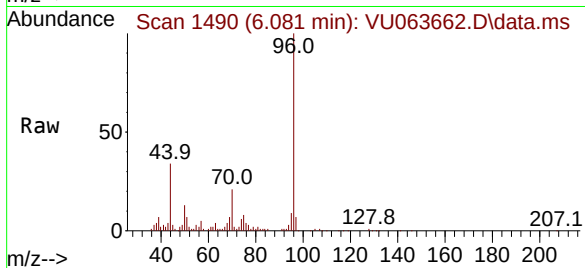

#57
4-Bromofluorobenzene
Concen: 0.917 ug/l
RT: 10.611 min Scan# 2899
Delta R.T. 0.003 min
Lab File: VU063662.D
Acq: 31 Oct 2025 15:29


Tgt Ion:	95	Resp:	24052
Ion Ratio	Lower	Upper	
95	100		
174	74.4	59.9	89.9
176	74.2	58.8	88.2

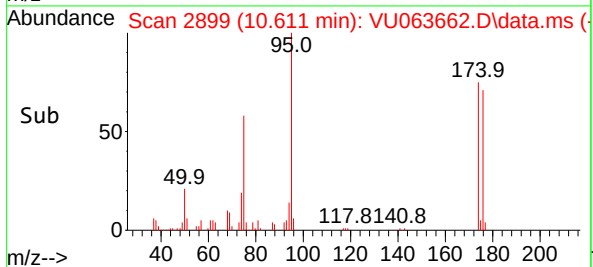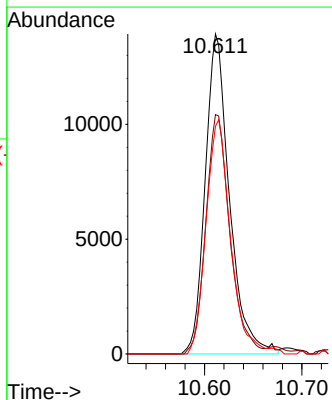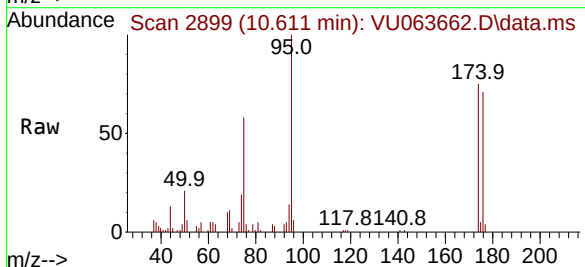

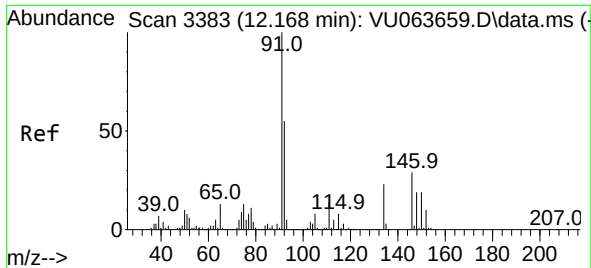

#68
1,2-Dichlorobenzene-d4
Concen: 0.931 ug/l
RT: 12.171 min Scan# 31
Delta R.T. 0.003 min
Lab File: VU063662.D
Acq: 31 Oct 2025 15:29

Instrument :
MSVOA_U
ClientSampleId :
VU1031WBL01

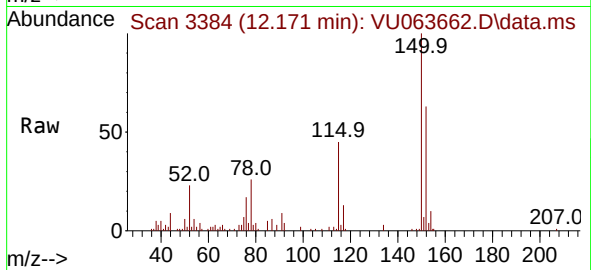

Tgt Ion:	152	Resp:	21876
Ion	Ratio	Lower	Upper
152	100		
115	69.7	0.0	247.2
150	159.0	0.0	643.6

