

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
 Data File : VU063664.D
 Acq On : 31 Oct 2025 16:59
 Operator : MD/SY
 Sample : Q2552-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063664.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.557	384	394	406	rBV	173037	273713	10.09%	1.080%
2	3.013	524	536	555	rBV	340030	627000	23.12%	2.474%
3	3.158	573	581	595	rVB	35882	77814	2.87%	0.307%
4	3.319	619	631	650	rBV	340355	670009	24.71%	2.644%
5	4.631	1027	1039	1055	rBV	127580	285103	10.51%	1.125%
6	5.277	1225	1240	1264	rBV	523780	1187875	43.80%	4.688%
7	5.486	1295	1305	1324	rVB3	66761	149623	5.52%	0.590%
8	5.740	1370	1384	1418	rBV2	612392	1715179	63.25%	6.769%
9	6.081	1481	1490	1506	rVB	60161	115386	4.26%	0.455%
10	6.508	1609	1623	1659	rBV	494877	1021528	37.67%	4.031%
11	6.762	1687	1702	1731	rBV	649468	1291070	47.61%	5.095%
12	7.942	2055	2069	2091	rBV	179047	337749	12.46%	1.333%
13	8.377	2191	2204	2233	rBV	641641	1146361	42.27%	4.524%
14	8.524	2237	2250	2276	rBV	756923	1347557	49.69%	5.318%
15	9.422	2515	2529	2550	rBV	1440675	2504557	92.36%	9.884%
16	9.544	2556	2567	2594	rVB	1638098	2711753	100.00%	10.701%
17	9.669	2594	2606	2643	rVB	1236165	2166717	79.90%	8.550%
18	10.077	2719	2733	2762	rBV2	1440777	2646318	97.59%	10.443%
19	10.460	2840	2852	2866	rVB	26454	43343	1.60%	0.171%
20	10.611	2884	2899	2914	rBV	72705	122171	4.51%	0.482%
21	10.881	2973	2983	2994	rBV	63305	99449	3.67%	0.392%
22	11.071	3031	3042	3060	rVB5	26244	52900	1.95%	0.209%
23	11.618	3202	3212	3225	rBV3	26104	41808	1.54%	0.165%
24	11.769	3251	3259	3263	rVV2	37031	50707	1.87%	0.200%
25	11.814	3263	3273	3296	rVB	625231	1034729	38.16%	4.083%
26	12.187	3370	3389	3409	rBV2	608690	1122175	41.38%	4.428%
27	13.814	3882	3895	3919	rBV	1457508	2428403	89.55%	9.583%
28	14.068	3964	3974	3991	rVB2	18584	35808	1.32%	0.141%
29	14.306	4037	4048	4067	rVB3	18810	33707	1.24%	0.133%




Sum of corrected areas: 25340512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063664.D
Acq On : 31 Oct 2025 16:59
Operator : MD/SY
Sample : Q2552-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

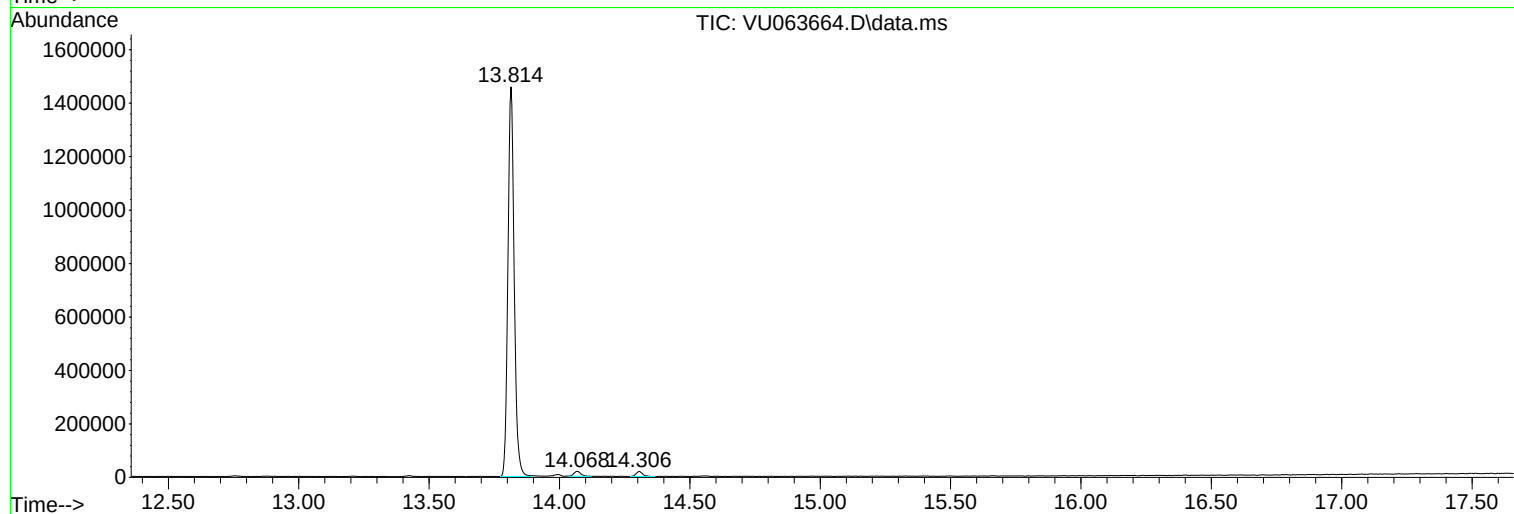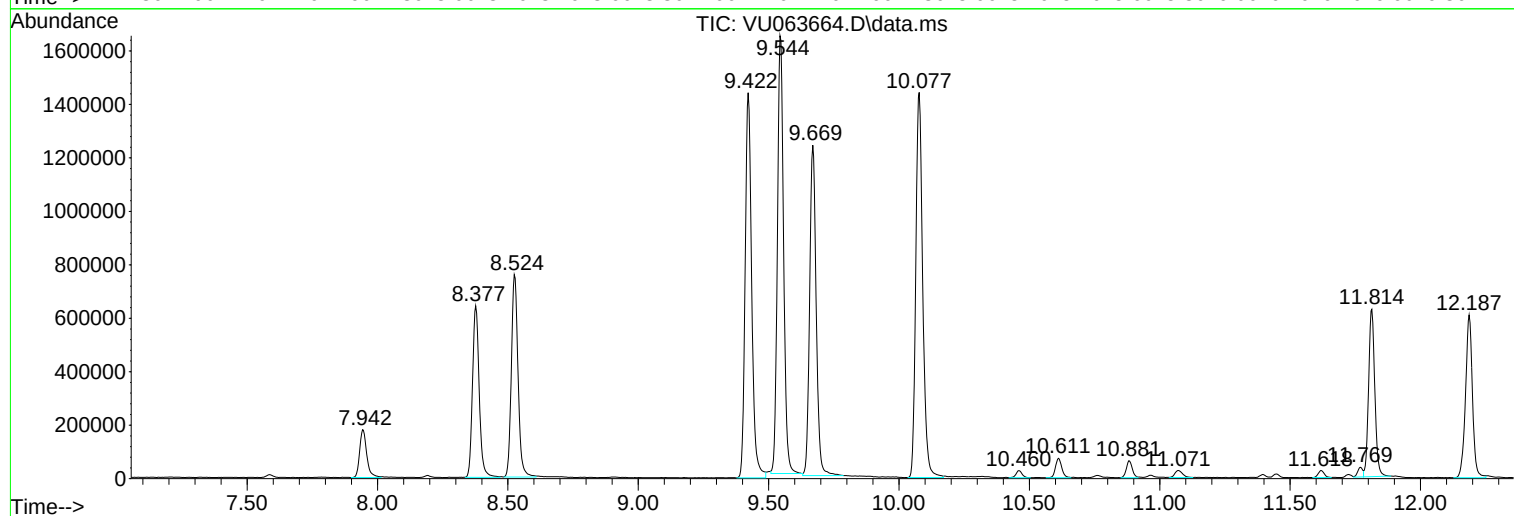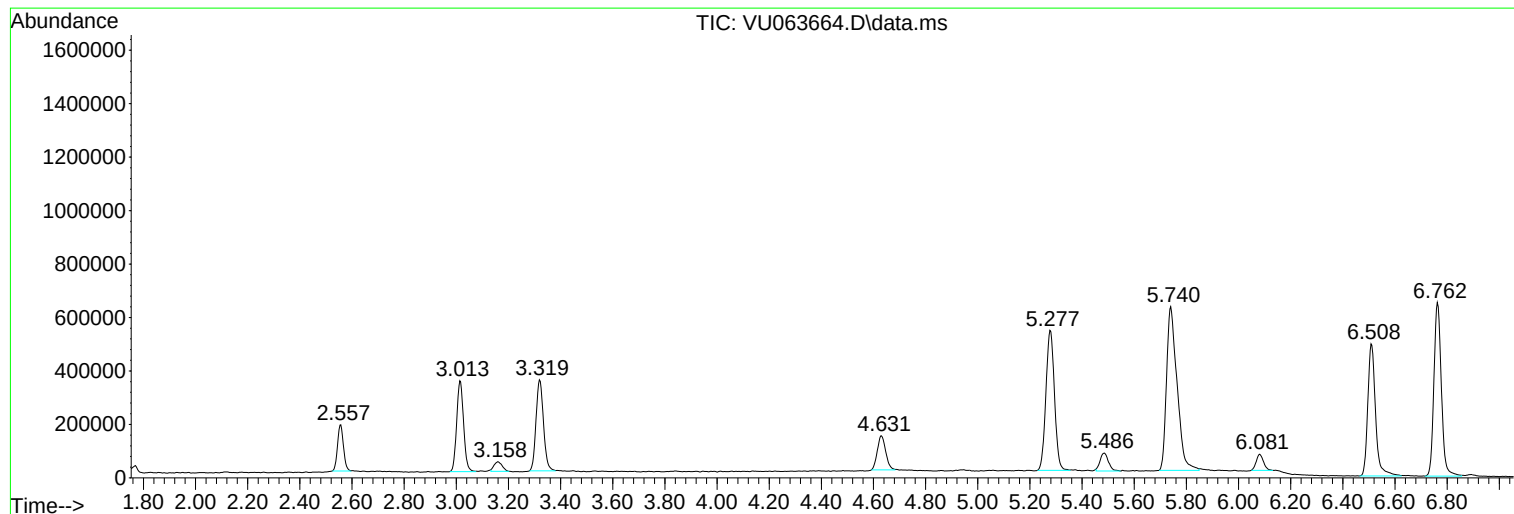

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063664.D
Acq On : 31 Oct 2025 16:59
Operator : MD/SY
Sample : Q2552-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063664.D
Acq On : 31 Oct 2025 16:59
Operator : MD/SY
Sample : Q2552-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------