

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
 Data File : VU063665.D
 Acq On : 31 Oct 2025 17:30
 Operator : MD/SY
 Sample : Q2552-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 WS0725-PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.830	160	168	183	rVB	84128	114826	1.92%	0.210%
2	2.117	246	257	274	rBV	1465936	2195318	36.65%	4.023%
3	3.158	571	581	598	rVB2	70644	163220	2.72%	0.299%
4	3.342	621	638	662	rBV	1923412	4420813	73.79%	8.102%
5	3.830	777	790	813	rVB	202374	478468	7.99%	0.877%
6	4.625	1021	1037	1061	rBV	567097	1397244	23.32%	2.561%
7	4.936	1120	1134	1152	rBV	410906	884079	14.76%	1.620%
8	5.486	1292	1305	1345	rBV	563421	1232752	20.58%	2.259%
9	6.078	1479	1489	1507	rVB	63325	132438	2.21%	0.243%
10	6.512	1612	1624	1637	rBV2	45985	95243	1.59%	0.175%
11	6.891	1729	1742	1771	rVB	414024	789890	13.19%	1.448%
12	7.583	1943	1957	1986	rBV	891973	1597518	26.67%	2.928%
13	8.187	2133	2145	2175	rBV	617610	1053881	17.59%	1.931%
14	8.550	2238	2258	2285	rBV2	184198	425406	7.10%	0.780%
15	9.422	2516	2529	2542	rBV	54069	100430	1.68%	0.184%
16	9.509	2543	2556	2586	rVV2	1437210	2525730	42.16%	4.629%
17	9.673	2594	2607	2623	rVB	69916	125950	2.10%	0.231%
18	10.078	2722	2733	2755	rBV2	63615	119992	2.00%	0.220%
19	10.460	2837	2852	2877	rBV	1151486	1883120	31.43%	3.451%
20	10.611	2888	2899	2924	rVB2	73478	140033	2.34%	0.257%
21	10.756	2931	2944	2952	rBV	1100350	1802963	30.10%	3.304%
22	10.798	2952	2957	2970	rVV	437515	678384	11.32%	1.243%
23	10.882	2970	2983	2998	rVV	2737035	4320292	72.12%	7.918%
24	10.962	2998	3008	3025	rVV	387423	690543	11.53%	1.266%
25	11.068	3029	3041	3072	rVB3	1367860	2430660	40.57%	4.455%
26	11.393	3124	3142	3150	rBV	831018	1309406	21.86%	2.400%
27	11.444	3150	3158	3171	rVB	636789	973781	16.25%	1.785%
28	11.618	3198	3212	3228	rBV	2042459	3207729	53.55%	5.879%
29	11.721	3231	3244	3250	rBV	737661	1168955	19.51%	2.142%
30	11.769	3250	3259	3271	rVB	2800171	4212155	70.31%	7.720%
31	12.184	3373	3388	3404	rBV	1749889	2749201	45.89%	5.039%
32	13.814	3874	3895	3913	rVB2	170252	332984	5.56%	0.610%
33	13.994	3935	3951	3962	rBV	3837792	5990669	100.00%	10.979%
34	14.061	3962	3972	3994	rVB	691396	1193202	19.92%	2.187%
35	14.303	4033	4047	4065	rBV	2205086	3625638	60.52%	6.645%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063665.D
Acq On : 31 Oct 2025 17:30
Operator : MD/SY
Sample : Q2552-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER




Sum of corrected areas: 54562913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063665.D
Acq On : 31 Oct 2025 17:30
Operator : MD/SY
Sample : Q2552-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

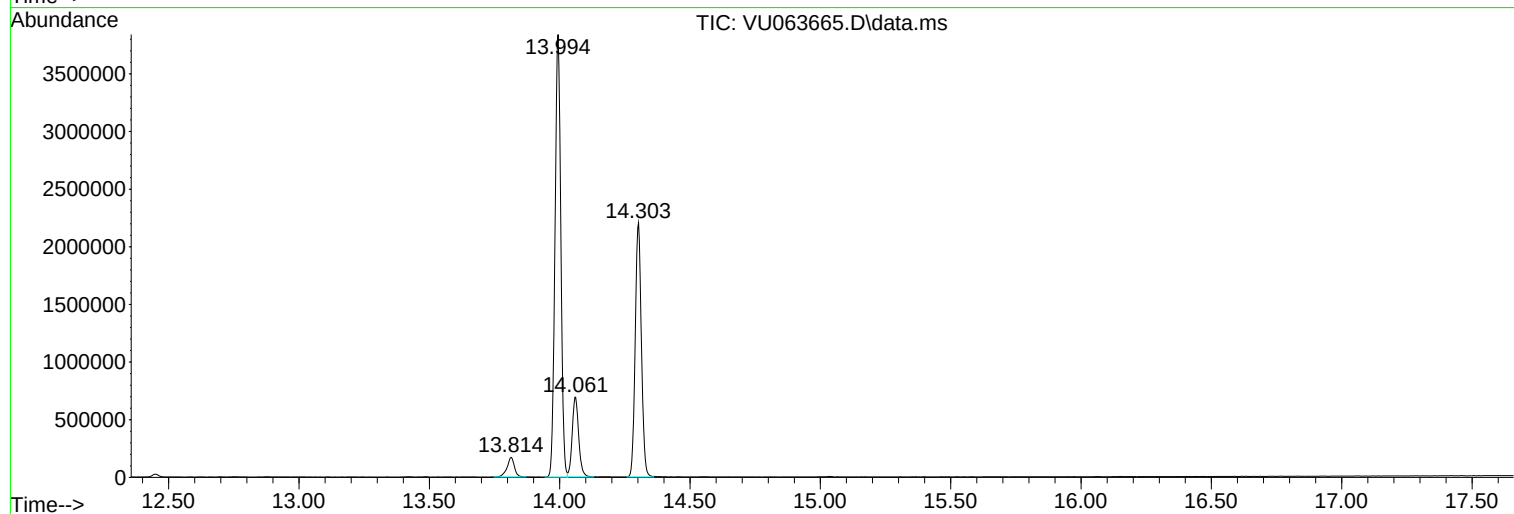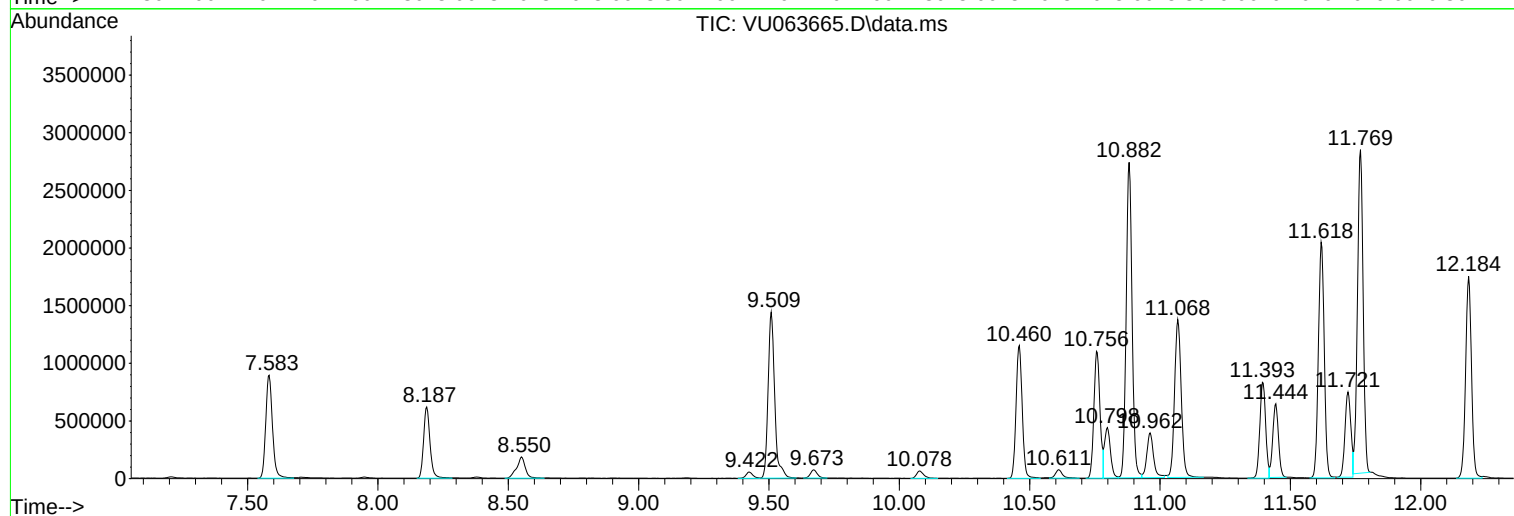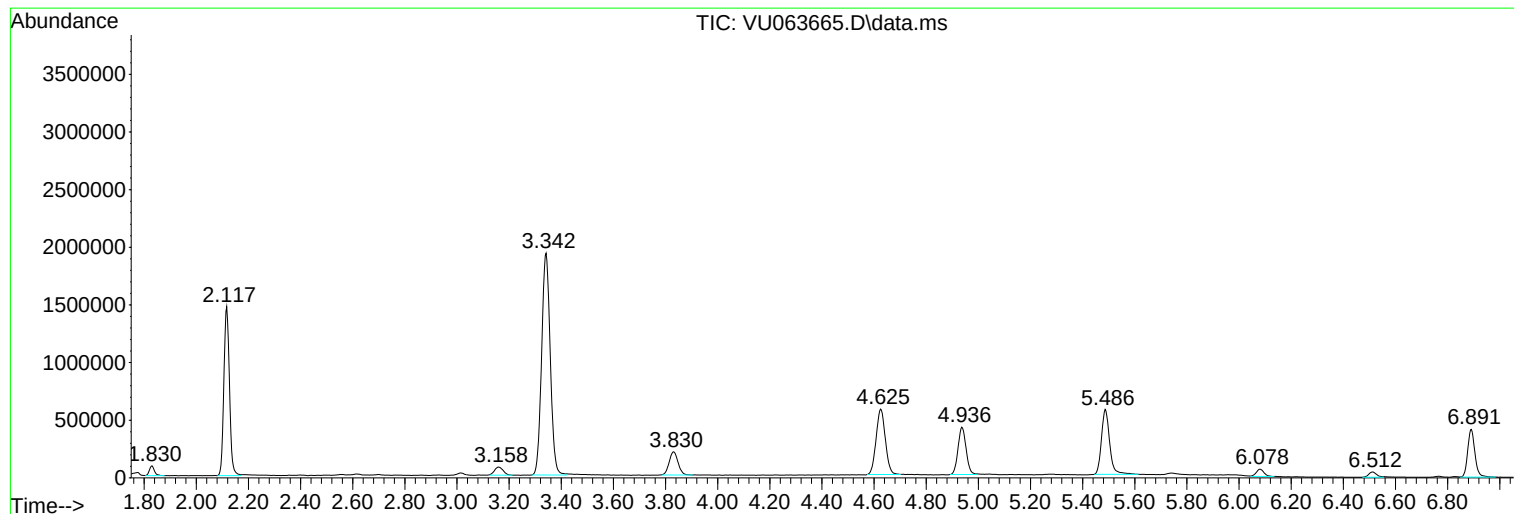

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063665.D
Acq On : 31 Oct 2025 17:30
Operator : MD/SY
Sample : Q2552-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063665.D
Acq On : 31 Oct 2025 17:30
Operator : MD/SY
Sample : Q2552-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
WS0725-PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------