


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU103125\
Data File : VU063654.D
Acq On : 31 Oct 2025 08:26
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Mon Nov 03 00:51:51 2025

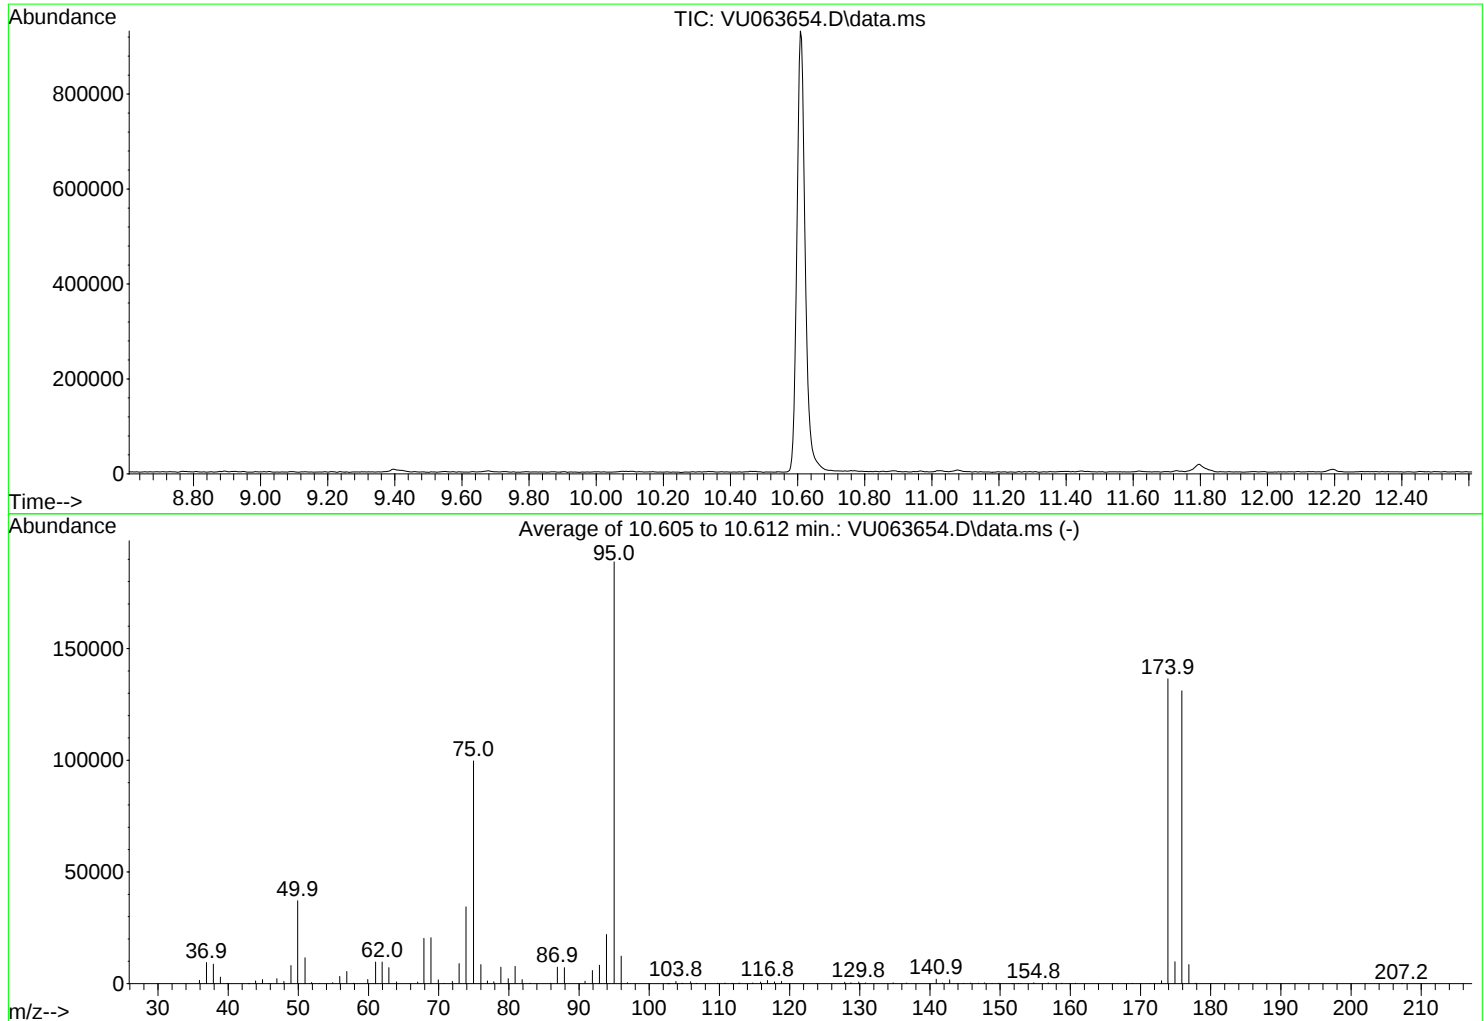

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	37099	PASS
75	95	30	60	52.8	99733	PASS
95	95	100	100	100.0	188843	PASS
96	95	5	9	6.5	12310	PASS
173	174	0.00	2	0.9	1269	PASS
174	95	50	100	72.3	136491	PASS
175	174	5	9	7.2	9832	PASS
176	174	95	101	96.0	131080	PASS
177	176	5	9	6.5	8562	PASS